Operation & Service Manual

Model 8311
SmartStep® Programmable Attenuator Units w/Ethernet

This documentation may not be reproduced in any form, for any purpose unless authorized in writing by Aeroflex / Weinschel, Inc.

AEROFLEX WEINSCHEL

© Aeroflex / Weinschel, Inc.
Frederick, Maryland
2008-2011

SAFETY SUMMARY

DEFINITIONS.

The following definitions apply to WARNINGS, CAUTIONS, and NOTES found throughout this manual.

WARNING

An operating or maintenance procedure, practice, statement, condition, etc., which, if not strictly observed, could result in injury and/or death of personnel. Do not proceed beyond a WARNING symbol until all the indicated conditions have been fully understood and/or met.

CAUTION

An operating or maintenance procedure, practice, statement, condition, etc., which, if not strictly observed, could result in damage or destruction of the equipment or long-term health hazards to personnel. Do not proceed beyond a CAUTION symbol until all the indicated conditions have been fully understood and/or met.

NOTE

An essential operating or maintenance procedure, condition, or statement that must be highlighted.

GENERAL PRECAUTIONS.

The following are general precautions that are not related to any specific procedure and, therefore, do not appear elsewhere in this publication. These are precautions that personnel must understand and apply during various phases of instrument operation or service.

WARNING

- Potentially lethal voltages are present in this instrument. Serious shock hazards from voltages above 70 volts may exist in any connector, chassis, or circuit board. Observe the following precautions:
- To minimize shock hazard, the instrument chassis must be connected to an electrical ground. Using the supplied three-conductor power cable ensures that the instrument can be firmly connected to the ac power source and electrical ground at a grounded power outlet. If using a 3-2 wire adapter be sure to connect the ground lead to earth ground.
- Use the buddy system any time work involving active high voltage components is required. Turn OFF the power before making/breaking any electrical connection. Regard any exposed connector, terminal board, or circuit board as a possible shock hazard. DO NOT replace any component or module with power applied.
- If test conditions to live equipment are required, ground the test equipment before probing the voltage or signal to be tested.
- Personnel working with or near high voltage should be familiar with modern methods of resuscitation.
- DO NOT wear jewelry (rings, bracelets, metal watches, and/or neck chains) while working on exposed equipment. Be very cautious about using hand tools near exposed backplanes, bus bars, and/or power supply terminals. Use properly insulated tools. When making test connections to the power supply terminals and bus bars, use only insulated probe tips.
- Verify that the instrument is set to match the available line voltage and the correct fuse is installed.
- DO NOT install substitute parts or perform any unauthorized modification to this instrument. Contact Weinschel Corporation to acquire any information on replacement parts or returning the instrument for repair. Unauthorized modification can cause injury to personnel and/or destruction of the instrument.
- Operating personnel must not remove instrument covers. Component replacement or adjustments MUST BE performed by qualified service personnel.
- DO NOT operate the instrument near or in the presence of flammable gases or fumes.

DETAILED PRECAUTIONS.

The following WARNINGS, CAUTIONS and NOTES appear throughout the text of this manual and are repeated here for emphasis.

CAUTION

- All procedures and/or steps identified as must be followed exactly as written and according to industry accepted ESDS device handling procedures. Failure to comply WILL RESULT in ESDS damage.
- DO NOT use a nylon bristle brush in the solvent as the bristles may dissolve and cause damage to the circuit card or component.
- DO NOT use ultrasonic cleaning on parts or assemblies containing electrical or electronic components.
- DO NOT bend pins of electrical connectors when using fiber-bristle brush.
- Compressed air used for cleaning and/or drying can create airborne particles that may enter the eye. Goggles/faceshields should be worn. DO NOT direct air stream towards self or other personnel. Pressure should be restricted to a maximum of 15 psi to avoid personal injury.
- Under no circumstances should a wire brush, steel wool, or abrasive compound be used on any surface. Using these items will cause extensive damage to the instruments surface.

NOTE

DO NOT return any instrument or component to Weinschel Corporation without receiving prior factory authorization.

SAFETY SYMBOLS.

The following symbols are used to identify safety hazards found throughout this publication and/or located on the instrument.

CAUTION
HIGH VOLTAGE





TABLE OF CONTENTS

1. GENERAL INFORMATION 5

1-1. PURPOSE 5
1-2. SCOPE 5
1-3. EQUIPMENT DESCRIPTION 5
1-4. USING THE MODEL 8310-XX-X-XN 5
1-5. UNPACKING AND INSPECTION 6
1-6. RESHIPMENT INSTRUCTIONS 6
1-7. STORAGE INSTRUCTIONS 6
1-8. RELATED MANUALS 7
1-9. ELECTROSTATIC DISCHARGE SENSITIVE (ESD) 7
1-10. ABBREVIATIONS & ACRONYMS 7
1-11. SAFETY CONSIDERATIONS 7
1-12. POWER REQUIREMENTS 7
1-13. ENVIRONMENTAL REQUIREMENTS 7

2. SPECIFICATIONS 8

2-1. GENERAL SPECIFICATIONS 8
2-2. CONFIGURATIONS\RF SPECIFICATIONS 8

3. INSTALLATION 9

3-1. RACKMOUNTING 9
3-2. INTIAL SETUP 9
3-3. INPUT/OUTPUT OPTIONS 9
3-3.1. POWER ENTRY MODULE ASSEMBLY 10
3-3.2. CHANNEL PORT CONNECTORS 10
3-3.3 MODE SELECT SWITCH 10

4. FRONT PANEL CONTROLS & INDICATORS 11

5. REMOTE OPERATION 12

5-1 COMMUNICATIONS INTERFACE 12-13
5-1.1. OPERATING MODES 13
5-1.2 SERIAL PORT SETUP 13
5-1.3 ETHERNET SETUP 13
5-1.3.1 DEVICEINSTALLER 13
5-1.3.2 SERIAL PORT LOGIN 14
5-1.3.3 ARP AND TELNET 15
5-1.3.4 DHCP 15
5-1.3.5 AUTOIP 15-16
5-1.3.6 BOOTP 16
5-1.3.7 DEVICE SERVER SETUP 16
5-1.3.8 EXAMPLE SETUP USING THE SERIAL PORT 16-20
5-2. SERIAL OPERATION 20-21
5-2.1. RS-232 OPERATION 21
5-3. STATUS REPORTING 22-23

5-4. GENERAL SYNTAX STRUCTURE 23-24
5-4.1. SYNTAX OF QUERIES 23
5-4.2. SYNTAX OF COMMANDS 23
5-4.3. OUTPUT DATA FORMAT 24
5-4.4. NOTATIONAL CONVENTION 24
5-5. COMMON COMMANDS 25-26
5-6 GENERAL COMMANDS 27-28

6. MAINTENANCE 29

6-1. INSPECTION 29
6-2. PREVENTIVE MAINTENANCE 29
6-3. SPECIAL CLEANING INSTRUCTIONS 29
6-3.1. MICROWAVE COAXIAL CABLE ASSEMBLIES 30
6-3.2. CIRCUIT CARDS AND MODULES 30
6-3.3. MACHINED SURFACES AND HARDWARE 30
6-3.4. CHASSIS CLEANING 30
6-3.5. CONNECTOR CLEANING 30
6-4. LINE VOLTAGE FUSE REPLACEMENT 31

7. REPLACEABLE PARTS LIST 32

7-1. UNDERSTANDING REFERENCE DESIGNATORS 32
7-2. ORDERING INFORMATION 32
7-3. DRAWING NUMBER 32
7-4. REPLACAEBLE PARTS LIST 32
7-4.1. REFERENCE DESIGNATOR 32
7-4.2. DESCRIPTION 32
7-4.3. PART NUMBER 32
7-4.4. VENDOR PART NUMBER 32
7-5.5. CAGE CODE 32
7-4.6. ASSEMBLY AND COMPPONET LOCATION 32
MODEL 8310-38-6-FN, ATTENUATOR UNIT ASSEMBLY REPLACEABLE PARTS LIST (P/N 193-7302-3) 33
MODEL 8310-38-6-RN, ATTENUATOR UNIT ASSEMBLY REPLACEABLE PARTS LIST (P/N 193-7302-4) 34
MODEL 8310-38-6-R-EN, ATTENUATOR UNIT ASSEMBLY REPLACEABLE PARTS LIST (P/N 193-7302-13) 35
MODEL 8310-202-2-FN, ATTENUATOR UNIT ASSEMBLY REPLACEABLE PARTS LIST (P/N 193-7305-4) 36
MODEL 8310-202-3-FN, ATTENUATOR UNIT ASSEMBLY REPLACEABLE PARTS LIST (P/N 193-7305-5) 37
MODEL 8310-202-2-RN, ATTENUATOR UNIT ASSEMBLY REPLACEABLE PARTS LIST (P/N 193-7305-6) 38
MODEL 8310-202-3-RN, ATTENUATOR UNIT ASSEMBLY REPLACEABLE PARTS LIST (P/N 193-7305-7) 39
MODEL 8310-352-6-FN, ATTENUATOR UNIT ASSEMBLY REPLACEABLE PARTS LIST (P/N 193-7307-2) 40
MODEL 8310-352-9-TN, ATTENUATOR UNIT ASSEMBLY REPLACEABLE PARTS LIST (P/N 193-7307-9) 41
MODEL 8310-352-12-TN, ATTENUATOR UNIT ASSEMBLY REPLACEABLE PARTS LIST (P/N 193-7307-13) 42
BASIC MODEL 8311-XX-X-XN (+5 V) ASSEMBLY REPLACEABLE PARTS LIST (P/N 193-81380 43
BASIC MODEL 8311-XX-X-XN ASSEMBLY REPLACABLE PARTS LIST (P/N 193-8138-1) 44

8. ACCESSORIES 45

9. CONTACTING AEROFLEX / WEINSCHEL. 45

10. AEROFLEX / WEINSCHEL WARRANTY 45

11. ASSEMBLY/WIRING DIAGRAMS

MODEL 8310-38-6-FN, ATTENUATOR UNIT ASSEMBLY DIAGRM 193-7302-3B
MODEL 8310-38-6-RN, ATTENUATOR UNIT ASSEMBLY DIAGRM 193-7302-4B
MODEL 8310-38-6-R-EN, ATTENUATOR UNIT ASSEMBLY DIAGRM 193-7302-13B
MODEL 8311-38-X-N ATTENUATOR UNIT ASSEMBLY WIRING DIAGRAM 193-8150A
MODEL 8310-202-X-FN, ATTENUATOR UNIT ASSEMBLY DIAGRAM ..... 193-7305-4, -5A
MODEL 8310-202-X-RN, ATTENUATOR UNIT ASSEMBLY DIAGRAM ..... 193-7305-6, -7A
MODEL 8310-202-X-XN, ATTENUATOR UNIT ASSEMBLY WIRING DIAGRAM 193-8148A
MODEL 8310-352-6-FN, ATTENUATOR UNIT ASSEMBLY DIAGRAM 193-7307-2A
MODEL 8310-352-9-TN, ATTENUATOR UNIT ASSEMBLY DIAGRAM 193-7307-9B
MODEL 8310-352-12-TN, ATTENUATOR UNIT ASSEMBLY DIAGRAM 193-7307-12A
MODEL 8310-352-6-FN, ATTENUATOR UNIT ASSEMBLY WIRING DIAGRAM 193-8141B
MODEL 8310-352-9-TN, ATTENUATOR UNIT ASSEMBLY WIRING DIAGRAM 193-8152A
BASIC MODEL 8311-XX-X-XN (+15 V) ASSEMBLY DIAGRAM 193-8138-1A
BASIC MODEL 8311-XX-X-XN (+15 V) ASSEMBLY WIRING DIAGRAM 193-8140A
ICD, SPECFICATIONS MODEL 8310-38-X-N 089-4157B
ICD, SPECFICATIONS MODEL 8310-202-X-XN 089-4090A
ICD, SPECFICATIONS MODEL 8310-352-X-XN 089-4073C
ICD, SPECFICATIONS MODEL 8310-352-9-XN 089-4193A
ICD, SPECFICATIONS MODEL 8310-352-9-XN 089-4255A

1. GENERAL INFORMATION:

1-1 PURPOSE: This manual contains setup and operation information for the Aeroflex / Weinschel's Model 8311-XX-X-XN Series of S*martStep*® Attenuator Units. The manual also provides component location, reference designators, part numbers, and nomenclature to identify all the assemblies and sub-assemblies of the Attenuator Unit.

1-2 SCOPE: This manual is to be used in conjunction with the operation and maintenance of a Model 8311-XX-X-XN Series S*martStep*™ Attenuator Unit. The manual also provides a description of each assembly; assembly parts list; block diagrams: and general maintenance procedures to maintain the instrument.

1-3 EQUIPMENT DESCRIPTION: Aeroflex / Weinschel's Model 8311-XX-X-XN Series SmartStep Attenuator Units represents a new concept in programmable attenuation for bench test and subsystem applications. Standard Model 8311-XX-X-XN designs house and control various Weinschel Programmable Attenuator Models (3200T, 150T, and 4200 Series) via front panel controls or standard communications interfaces including Ethernet and RS-232 Serial. Special configurations also exists where the RF section is designed to specific customer requirements which can contain to multiple programmable attenuations used in conjunction with other coaxial devices such as switches, power combiners, directional couplers, and filters creating single or multi-channel subsystems.

1-4 USING THE MODEL 8310-XX-X-XN: The Model 8311-XX-X-XN Series provides front-panel and computer control for up to 12 channels of attenuation, RF switching, or other functions. The Model 8311-XX-X-XN combines the features of the Aeroflex / Weinschel 8210A Device Controller with a front panel user interface to form a flexible, easy to use solution. Most Model 8311-XX-X-XN Series are multi-channel configurations where RF signal is routed through either the front or rear mounted channel connector to a single or multiple Weinschel programmable attenuators thus creating a channel.

For specialized configurations refer to supplemental information in the front of this manual for details. Typically Weinschel programmables are bi-directional and the RF signal can be applied to either Channel connector. Channels can be selected by selecting the front panel CHAN button. When selected, as indicated by the CHAN indicator, a new attenuation value may be entered using the INCR and DECR keys. The main display will show the current attenuation setting of the channel.

A new attenuation setting in dB may be entered using the INCR/DECR or ENTRY keys. The front panel STEP key allows the user to define the attenuation step size used by the INCR and DECR keys. Remember that the attenuation step size (resolution) is limited to the physical size of the internal attenuator cells. For example a 0-70 unit with 10 dB steps can only be adjusted in 10 dB increments but larger increments such as 20, 30, 40 dB can be set using this key. The REL key allows the user to set relative mode for attenuators.

When turned on, the currently displayed attenuation value is used as a reference value from which the attenuation may be set. In this mode, attenuation values may be positive or negative from the reference setting. When REL is turned off, the display returns to the actual attenuation setting for the channel. Refer to Section 5 for more detailed information about the front panel keys and indicators. All Model 8311-XX-X-XN Series functions can also be controlled via standard communications interfaces including Ethernet and RS-232 Serial. Refer to Section 6 for bus setup and operating instructions when using the Model 8311-XX-X-XN Series in the remote mode.

1-5. UNPACKING AND INSPECTION: Upon unpacking the equipment, retain the shipping container and packing material for future shipment for recalibration. Perform the following initial inspection:

a. Carefully look at the outside of the shipping container for discoloration, stains, charring, or other signs of exposure to excessive heat, moisture, or liquid chemicals. Check for any physical damage to the shipping container such as dents, snags, rips, crushed sections or areas, or similar signs of excessive shock or careless handling.

b. With the equipment and any accessory package removed from the shipping container, check each item against the packing list or Items Supplied List. If any items are missing, contact the Weinschel, Inc. Customer Service Department.

c. Carefully inspect the equipment looking for dents, deep scratches, damaged or loose connector, or any other

d. signs of physical abuse or careless handling. If damage is found, forward an immediate request to the delivering carrier to perform an inspection and prepare a concealed-damage report. DO NOT destroy any packing material until it has been examined by an agent of the carrier. Concurrently, report the nature and extent of damage to Weinschel, Inc., giving equipment model and serial numbers, so that necessary action can be taken. Under U.S. shipping regulations, damage claims must be collected by the consignee; DO NOT return the equipment to Aeroflex / Weinschel, Inc. until a claim for damages has been established.

1-6. RESHIPMENT: Use the best packaging materials available to protect the unit during storage or reshipment. When possible, use the original packing container and cushioning material. If the original packing materials are not available, use the following procedure:

a. Wrap the storage cases in sturdy paper or plastic;

b. Place the wrapped storage cases in a strong shipping container and place a layer of shock-absorbing material (3/4 inch minimum thickness) around all sides of the unit to provide a firm cushion and to prevent movement inside the container.

c. If shipping the unit for service, attach a tag to indicate:

1. model and serial numbers
2. service required
3. description of malfunction
4. return address
5. authorization to conduct repairs
6. return authorization number

d. Thoroughly seal the shipping container and mark it FRAGILE. Ship to:

Aeroflex / Weinschel, Inc.
Attn: Customer Service Department
5305 Spectrum Drive
Frederick, MD 21703-7362
or to an authorized sales representative.

1-7. STORAGE: Storage of the Model 8311-XX-X-XN Series *SmartStep*™ Attenuator Unit is possible for extended periods without incurring damage to internal circuitry if the Model 8311-XX-X-XN Series is packaged according to the instructions above. The safe limits for storage environment are as follows:

Temperature:	4° to +167 °F (-20° to +75 °C)
Humidity:	less than 95% without condensation
Altitude:	Up to 40,000 feet

1-8. RELATED MANUALS: The following manuals contain information that may be used in conjunction with this manual to operate, service, or calibrate this instrument.

Manual	Title
H4-1 and H4-2	Federal Supply Code for Manufacturers Cataloging Handbook
IM-275	Operating & Installation Instructions for 3200T & 3201T Series ***SmartStep*** Programmable Attenuators
IM-276	Operating & Installation Instructions for 150T, 151T, 152T & 152T Series ***SmartStep*** Programmable Attenuators
IM-248	Operating & Installation Instructions for 4226 & 4228 Series ***SmartStep*** Solid-State Programmable Attenuators
IM-425	Operating & Installation Instructions for 3206T & 3208T Series ***SmartStep*** Solid-State Programmable Attenuators

1-9. ELECTROSTATIC DISCHARGE SENSITIVE: The equipment documented in this manual contains certain Electrostatic Discharge Sensitive (ESDS) components or parts. Therefore, certain procedures/steps are identified by the use of the symbol . This symbol is used in two ways:

CAUTION

All procedures and/or steps identified as must be followed exactly as written and according to accepted ESDS device handling procedures. Failure to comply **WILL RESULT** in ESDS damage.

a. When the ESDS symbol is placed between a paragraph number and title , all of that paragraph, including all subparagraphs, is considered ESDS device handling procedure.

b. When the ESDS symbol is placed between a procedure/step number and the text , all of that procedure is considered an ESDS device handling procedure.

1-10. ABBREVIATIONS AND ACRONYMS: The following list contains abbreviations used throughout this manual. Abbreviations and acronyms that are not listed conform to MIL-STD-12D.

DUT	Device Under Test
ESDS	Electrostatic Discharge Sensitive
DIB	Device Interface Bus
TBD	To Be Determined

1-11. SAFETY CONSIDERATIONS: The Attenuator Unit and all related documentation must be reviewed for familiarization with safety markings and procedures before any operation and/or service. Refer to the SAFETY SUMMARY located at the beginning of this manual for a summary of safety information and procedures. Following these simple safety precautions will ensure safe operation and service of the Attenuator Unit.

1-12. POWER REQUIREMENTS: Aeroflex / Weinschel supplies a detachable power cable (P/N 068-21) to connect an 100 to 240 Vac power source with a frequency between 50 to 60 Hz to the Attenuator Unit. To minimize shock hazard, the instrument chassis must be connected to an electrical ground. Using the supplied three-conductor power cable ensures that the instrument can be firmly connected to the ac power source and electrical ground (safety ground) at a grounded power outlet. Refer to paragraph 4-2 (Initial Setup) before applying any power to the instrument**.**

1-13. ENVIRONMENTAL REQUIREMENTS: This instrument performs best within its specifications when operated within a controlled environment having an ambient temperature of 0°± 50°C, Relative Humidity of up to 95% non condensing, and a altitude of less than 40,000 feet. Operating beyond these limits can affect the accuracy and performance of the instrument and damage internal circuitry.

2. SPECIFICATIONS:

2-1. GENERAL SPECIFICATIONS:

Input Power Requirements	ac 115 to 230 Vac, 1.6 A, 50/60 Hz, 50 Watts
Environmental	Operating Temperature 0 to +50°C Storage Temperature: 4° to +167 °F (-20° to +75 °C)
RS-232 (Serial) Bus(1)	Connector: 9-pin male D Signals: TXD, RXD, RTS, CTS, DTR, GND Baud Rates: 2400, 9600, 19200, and 38400 Data Bits: 8 Handshaking: None, RTS/CTS, XON/XOFF Parity: None, Odd, Even Indicators: Tx (Transmit) and Rx (Receive)
Ethernet TC/IP	10/100 Base T Connector: Standard RJ45
RF Characteristics(3)	See Model Configuration Table below.

NOTES:
1. RS-232 can be used with standard PC serial port for short and medium distances (up to approximately 50 ft).
2. Refer to Individual data sheet (Appendix C) for detailed specifications on internal programmable attenuators.

2-3. CONFIGURATIONS\RF SPECIFICATIONS:

Model No	Attenuator Value	Frequency Range (GHz)	Insertion Loss	SWR	No. of Channels	Attenuator Type	Connector Type	Connector Location	Drawing Number
8311-1-6-FN	63/1	dc-1.0	6.00 dB max	1.6 max	6	3250T-63	BNC/F	Front	
8311-38-6-FN	63/1	dc-2.0	5.25 dB max	1.4 max	6	3206T-1	N/F	Front	193-7302-3
8311-38-6-RN	63/1	dc-2.0	5.25 dB max	1.4 max	6	3206T-1	N/F	Rear	193-7302-4
8311-38-6-R-EN	63/1	dc-2.0	5.25 dB max	1.4 max	6	3206T-1	N/F	Rear	193-7302-13
8311-38-12-TN	63/1	dc-2.0	5.25 dB max	1.4 max	6	3206T-1	N/F	Front-Rear	
8311-137-6-FN	63/1	dc-3.0	4.70 dB max	1.6 max	6	4226T-63	N/F	Front	
8311-137-6-RN	63/1	dc-3.0	4.70 dB max	1.6 max	6	4226T-63	N/F	Rear	
8311-202-2-FN	121/1	dc-18.0	3.25 dB max	1.95 max	2	150T-11, 150T-110	SMA/F	Front	193-7305-4
8311-202-3-FN	121/1	dc-18.0	3.25 dB max	1.95 max	3	150T-11, 150T-110	SMA/F	Front	193-7305-5
8311-202-2-RN	121/1	dc-18.0	3.25 dB max	1.95 max	2	150T-11, 150T-110	SMA/F	Rear	193-7305-6
8311-202-3-RN	121/1	dc-18.0	3.25 dB max	1.95 max	3	150T-11, 150T-110	SMA/F	Rear	193-7305-7
8311-204-6-FN	62/2	dc-18.0	3.25 dB max	1.95 max	6	150T-62	SMA/F	Front	
8311-352-6-FN	103/1	dc-6.0	6 dB max	1.55 max	6	3408T-103	SMA/F	Front	193-7307-2
8311-352-9-TN	103/1	dc-6.0	6 dB max	1.55 max	9	3408T-103	SMA/F	Front	193-7307-9
8311-352-12-TN	103/1	dc-6.0	6 dB max	1.55 max	9	3408T-103	SMA/F	Front	193-7307-12

3-1. RACKMOUNTING: Standard 8311 Attenuator Units are shipped with four plastic feet mounted to the bottom cover, this allows the user to place the instrument on any bench or to stack the with other Weinschel instruments. The Model 8311 can also be rack mounted as a using Rack Mounting Kit (P/N 193-8033-1). Using these kits will allow the Model 8310 to be mounted in any rack or cabinet that is designed according to EIA RS-310 or MIL-STD-189.

3-2. INITIAL SETUP: The following initial setup procedures should be performed prior to operating the 8311-XX-X-XN Attenuator Unit.

a. Perform inspection paragraph 1-4 prior to connecting the 8311-XX-X-XN to any power source.
b. Check that the external power source outputs to the 8311-XX-X-XN Series are in accordance with Section 2, Specifications.
c. Install the 8311-XX-X-XN Series into a cabinet or rack, if desired.
d. Using the supplied power cord connect the 8311-XX-X-XNto the external power source.
e. Setup the IEEE-488 bus address or other Communications options for your application using 5. If using the Ethernet configure the selectable Bus Select switch to Ethernet and refer to section 5 for operating instructions.

3-3 INPUT/OUTPUT OPTIONS: The following paragraphs provide a description of the connections that can be made to the 8311-XX-X-XNAttenuator Unit. Figure 2 shows the location of these connectors and switches.

WARNING

Sufficient power levels are present at the Power Input Assembly to cause personal injury. Ensure that the instrument power cord is DISCONNECTED before attempting to change fuses.

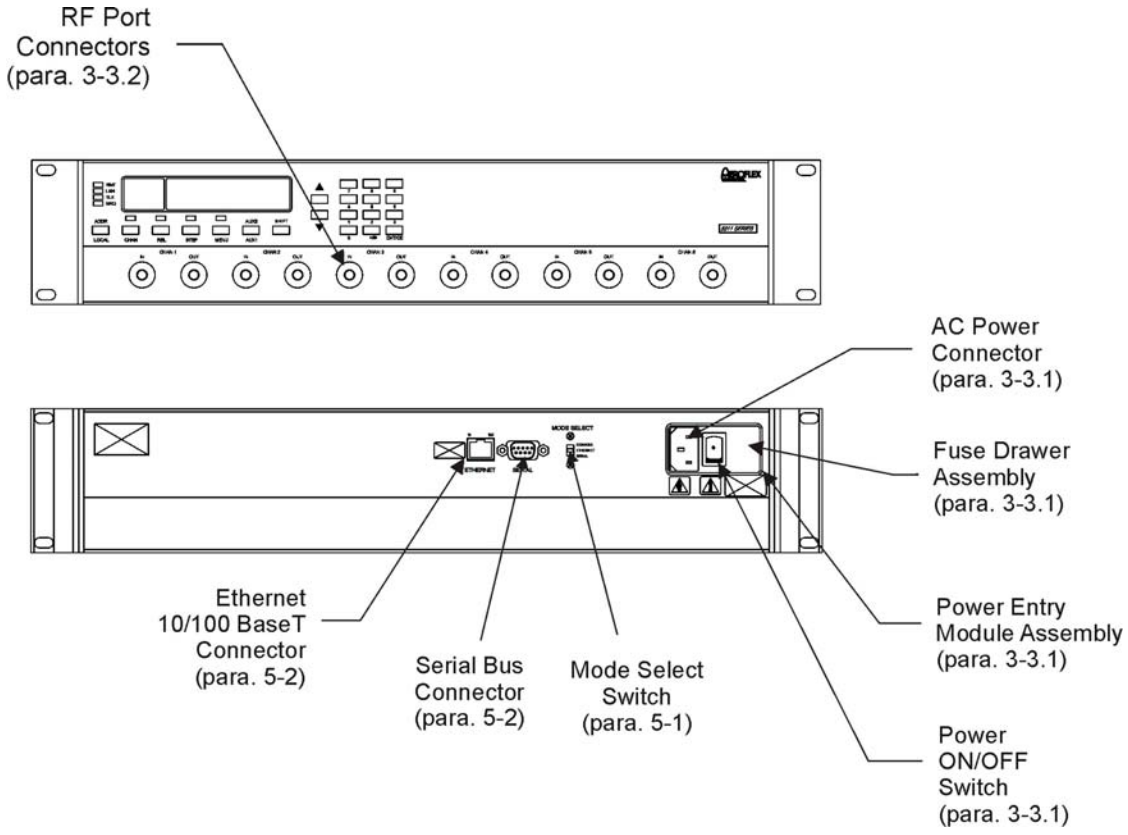
RF Port Connectors (para. 3-3.2)
AC Power Connector (para. 3-3.1)
Fuse Drawer Assembly (para. 3-3.1)
Power Entry Module Assembly (para. 3-3.1)
Power ON/OFF Switch (para. 3-3.1)
Ethernet 10/100 BaseT Connector (para. 5-2)
Serial Bus Connector (para. 5-2)
Mode Select Switch (para. 5-1)

Figure 1. Front & Rear Panel Connectors

3-3.1 POWER ENTRY MODULE ASSEMBLY: The Power Entry Module Assembly located on the rear panel contains a three-prong ac power input connector and a fuse drawer assembly (Figure 1). The **Fuse Drawer Assembly** contains the line voltage fuse (Weinschel P/N 052-1-1.5). The Model 8311-XX-X-XN uses a T 1.5A, 250 Vac fuse which is 5 x 20 mm in size. Refer to paragraph 6-4.1 for replacement of the fuse.

The **AC Power Connector**, located on the left side of XF1 (Figure 1), is a plug-type, prong insert connector with three conductors for connection of the power cord (P/N 068-21) to the Power Supply Assembly located within the Attenuator Unit. This connector also grounds the chassis of the Attenuator Unit when the the ac power cord is connected to a grounded wall outlet. If necessary, use a three prong to two prong adapter and connect the adapter's ground lead to the outlet plate retaining screw.

The **Power ON/OFF Switch** is located on the rear panel and in part of the Power Entry Module Assembly. Placing the POWER ON/OFF switch in the ON position applies power to the instrument.

CAUTION

When applying an RF signal to the RF INPUT connector, DO NOT exceed the maximum allowable power level specifications of the Model 8310-XX-X-XN.

3-3.2. CHANNEL PORT CONNECTORS: A typical Model 8311-XX-X-XN Series Attenuator Unit contains 12 standard D holes on the front and rear panel allowing for single or multichannel configurations. Standard Model 8311-XX-X-XN's are supplied with two PLANAR CROWN® Type N connectors that can be mounted on the front or rear panel. These connectors provide a input and output port where various types of RF signals can be applied to the devices internally mounted in the Model 8311-XX-X-XN (Connector location specified by customer when ordering). Some special configurations could contain Aeroflex / Weinschel's Model 1568 SMA Panel Adapters or other types of crowns (see accessories for other types).

NOTE

The use of the PLANAR CROWN® connectors provide the user with easy exchange of connector types, which eliminates the need for adapters and other devices that would create additional insertion loss. This type of connector also provides quick removal and replacement of defective connectors. For more information about the PLANAR CROWN® connectors contact the Sales Department at Aeroflex / Weinschel, Inc.

3-3.3. MODE SELECT SWITCH: This 3 position slide switch located on the rear panel, allows the user to select between Serial, Ethernet or Console Mode operation. Refer to paragraph 5-1 for more information about the different operational modes of the Model 8310-XXX-XN communication interface.

4. FRONT PANEL CONTROLS & INDICATORS:

The following paragraphs provide setup and general guidelines for operating the Model 8311-XX-X-XN Series ***SmartStep*** Attenuator Unit and its different bus configurations. Also provided is a general description of the internal circuitry of the Model 8310-XX-X-XN.

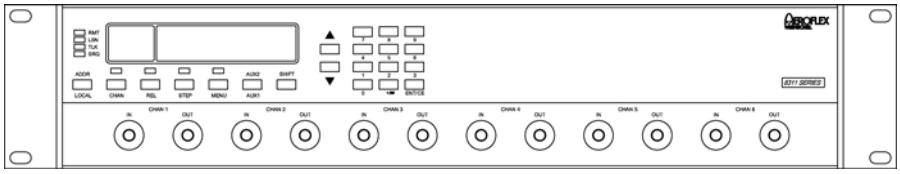

Figure 2. Model 8311-XX-X-XN Series Front Panel

ENTRY keys: The numeric entry keys allow the user to directly enter numeric values. When using the keypad, values are not updated until the ENT (enter) key is pressed. The Minus (-) and CE (clear entry) functions may be accessed via first depressing the SHIFT key.

INCR & DECR : The INCR and DECR keys allow settings to be scrolled from their current value. Unlike the ENTRY keys, the new setting is updated immediately without the use of the ENT key.

CHAN: Allows the selection of the current channel, as indicated by the CH1-CH4 indicators. Repeated depressions of the CHAN key will select the next available channel. The main display will show the current setting of the channel. For configurations with 5 or more channels, selecting the CHAN key will display the current selected channel in the main display. Channels are then selected via the INCR and DECR keys.

REL: This key control allows the use of a relative mode for attenuators, as indicated by the REL mode indicator. When turned on, the currently displayed attenuation value is used as a reference value from which the attenuation may be set. In this mode, attenuation values may be positive or negative from the reference setting. When REL is turned off, the display returns to the actual attenuation setting for the channel.

STEP: This key allows the user to change the attenuation step size used by the INCR and DECR keys. When turned on, as, indicated by the STEP indicator, the current step size is displayed in the main display, and a new value may be entered using the INCR/DECR or ENTRY keys. The step size may be set to any multiple of the intrinsic step size for the currently selected channel.

MENU: Invokes the menu functions. Menu selections may be made via the INCR and DECR keys. (NOTE: menu functions are currently not implemented as of 3/8/99)

AUX1/AUX2: The function of these keys is user-programmable via remote operation. They invoke any currently defined AUX1 and AUX2 macros. Refer to the macro programming section for information on creating macro definitions.

LOCAL: This key places the Model 8311 in local operation mode, unless the key function has been overridden via an IEEE-488.2 local lockout or execution of the LOCKOUT command.

ADDR: This key displays the current IEEE-488.2 address. The address may be changed from the front-panel, however, the initial setting at power on is derived from the rear-panel address switch.

5. REMOTE OPERATION:

The following paragraphs provide setup and general guidelines for operating the Model 8311 using an external controller.

5-1. COMMUNICATIONS INTERFACE: The unit provides for control via a number of interface methods, including IEEE 488.2, RS232 serial, and 10/100 baseT Ethernet. Interface functions are split between two assemblies:

1). the main controller (generically referred to as the 8210A),

2). the ethernet control interface.

The 8210A is responsible for control of the RF devices, and handles GPIB and RS232 communications. The Ethernet control interface utilizes a Lantronix XPort™ Ethernet to serial device server which allows the 10/100baseT Ethernet network to communicate to the 8210A via the RS232 port.

A block diagram of the communications subsystem is shown below.

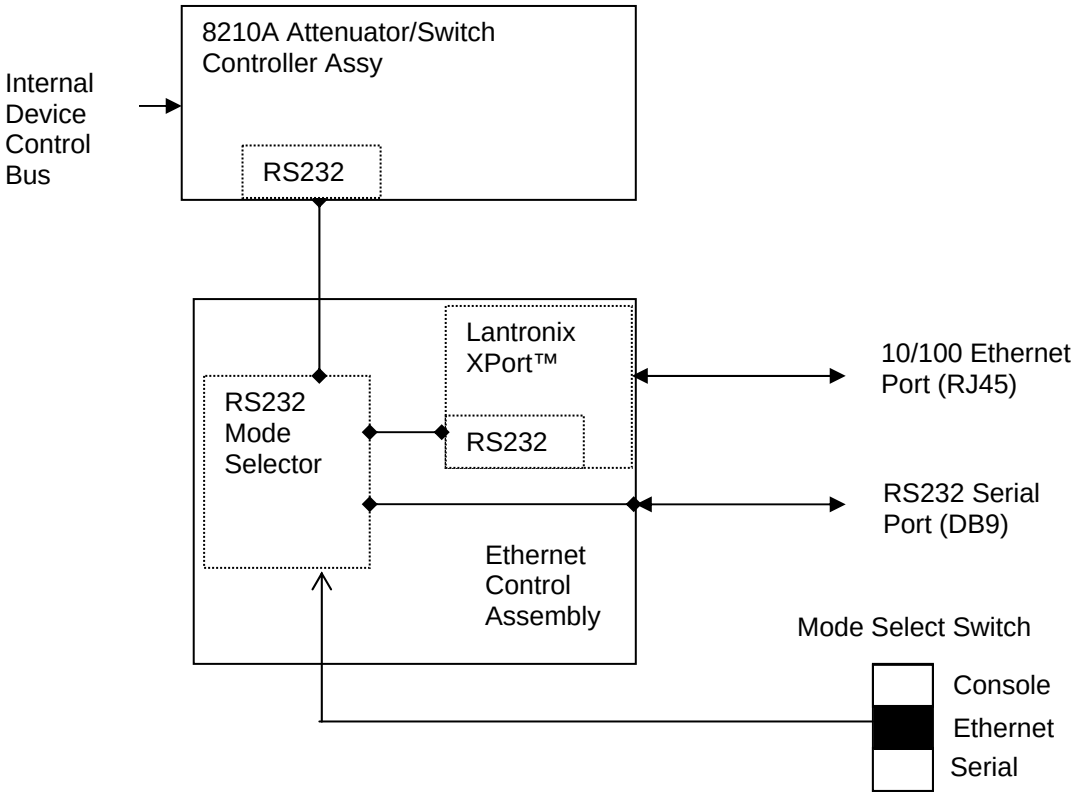

A copy of the Xport Users Guide and the Lantronix DeviceInstaller program is included on the provided CD.

For detailed information regarding the setup and operation of the XPort™ Device Server, consult the Lantronix documentation available at the Lantronix website www.lantronix.com

5-1.1 Operating Modes: The rear-panel RS232 port serves several functions, which are controlled via the 3-position Mode Select Switch.

Serial Mode: This position allows the RS232 port to be directly connected to the serial port of the 8210A, effectively bypassing the XPort's ability to control the unit via the Ethernet port. In this mode, the serial port settings are controlled via the internal DIP switch of the 8210A.

Ethernet Mode: This position internally connects the serial port of the device server to the serial port of the 8210A, allowing for network control of the unit. In this mode, the external serial port is non-functional. The serial communication settings of the device server must be set to match that of the 8210A for proper operation.

Console Mode: This position connects the RS232 port directly to the XPort device server. This mode allows the setup/configuration of the device server to be performed via the RS232 port. In this mode, serial communications are fixed at 9600 N81. For detailed information regarding operation, refer to the Xport Users Guide Chapters 5-8 (Setup Mode) and Chapter 11 (Monitor Mode).

5-1.2 Serial Port Setup: By default, the unit is shipped configured for 9600 baud, no parity, and 1 stop bit, with no handshaking required (9600N81). The rear-panel male DE-9 connector is configured as a DTE port (the same as a typical PC) with the following pinout:

Pin	Name	Dir	Description
2	RXD	←	Receive Data (in)
3	TXD	→	Transmit Data (out)
5	GND	--	System Ground

Connection to another DTE device (ie a PC) requires the use of a null-modem cable to swap pins 2 and 3.

Communication settings for the 8210A are controlled via the internal Serial/GPIB Settings DIP switch located on the board (refer to the 8210A Manual IM-288), while the XPort serial configuration is set independently and can be done using a variety of methods. Refer to the Xport Users Guide for a detailed description of the available setup mode methods and options.

NOTE

If you wish to change the serial port operation, keep in mind that the settings must match in both places in order for the XPort to communicate successfully with the 8210A when used in the Ethernet control mode.

5-1.3 Ethernet Setup: The network address of the XPort must be configured prior to use. There are several ways to assign an IP address to the Xport. A general overview is provided here. For more detailed information and links to video tutorials on performing many of these steps, refer to the information provided on the CD.

5-1.3.1 DeviceInstaller: The Lantronix DeviceInstaller is a Windows-based program that can be used to setup the Xport. Of the methods presented here, this is the simplest. However, the DeviceInstaller relies on the Xport being set for DHCP. If a static IP has been previously assigned to the Xport, there is a high probability that the DeviceInstaller will not be able to see the Xport, especially if the IP or Gateway network settings do not match that of the PC currently being used. If that is the case, you will have to use one of the other methods outlined below.

To use the DeviceInstaller utility, first install it from the product CD or click on the link below to download the latest version of DeviceInstaller.

http://ltxfaq.custhelp.com/app/answers/detail/a_id/644

a. Insert the product CD into your CD-ROM drive.

b. View Readme.txt located in the Lantronix Xport CD files Rev2 folder.

c. Select the desired DeviceInstaller and run the associated setup program within the folder.

d. Respond to the installation wizard prompts. (When prompted to select an installation type, select Typical.)

Assigning an IP Address in DeviceInstaller

a. Click Start->Programs->Lantronix->DeviceInstaller->DeviceInstaller. If your PC has more than one network adapter, a message displays. Select an adapter and click OK.

b. Click the Search icon and select the unit from the list of Lantronix device servers on the local network.

c. Click the Assign IP icon.

d. If prompted, enter the hardware address (on the product label) and click Next.

e. Select Assign a specific IP address and click Next.

f. Enter the IP address. The Subnet mask displays automatically based on the IP address; if desired, you may change it. On a local network, you can leave the Default gateway blank (all zeros). Click Next.

g. Click the Assign button and wait several seconds until a confirmation message displays. Click Finish.

h. Select the device from the main window list and select Ping from the Tools menu. The Ping Device dialog box shows the IP address of the selected unit.

i. From the Tools menu, click the Ping button. The results display in the Status window. Click the Clear Status button to clear the window so you can ping the device again.

> **Note:** If you do not receive “Reply” messages, make sure the unit is attached to the network properly and the IP address assigned is valid for the particular network segment you are working with. If you are not sure, check with your systems administrator.

j. Click the Close button to close the dialog box and return to the main window.

5-1.3.2 Serial Port Login: To assign the IP address and other network settings using a serial connection:

a. Connect a console terminal or a PC running a terminal emulation program to the rear-panel RS232 connector. The default serial port settings are 9600 baud, 8 bits, no parity, 1 stop bit, no flow control. Set the rear-panel Mode Select switch to the Console position.

b. To enter Setup Mode, cycle the unit's power (power off and back on). After power-up, the self-test begins and the red Diagnostic LED starts blinking. You have one second to enter three lowercase ‘x’ characters.

Note: The easiest way to enter Setup Mode is to hold down the ‘x’ key at the terminal (or emulation) while powering up the unit.

c. The display should be similar to:

MAC address 00204AC530DB
Software version V6.6.0.2 (080926) XPTEXE
Press Enter for Setup Mode

d. The Xport has a built-in timeout function, and you must press the ‘Enter’ key within three seconds to enter the Setup Mode. If you do not, the Xport will timeout and display “?!?”, after which it will continue with the boot process and you will have to repeat Step 2.

e. Select 0 (Server Configuration) and follow the prompts until you get to IP address.

f. Enter the new IP address, subnet mask, and gateway (if applicable).

g. Select 9 to save and exit Setup Mode. The unit performs a power reset.

5-1.3.3 ARP and Telnet: If a serial port is unavailable, you can use the Address Resolution Protocol (ARP) method from UNIX and Windows-based systems to assign a temporary IP address.

To assign a temporary IP address:

a. On a UNIX or Windows-based host, create an entry in the host's ARP table using the intended IP address and the hardware MAC address of the Xport, which should be available on the rear-panel of the unit. Make sure that the intended IP is reachable with the current network settings of the host. The following example uses an IP of 192.12.3.77. Substitute the desired address in it's place, and the MAC address of the Xport in place of the 00:20:4a:xx:xx:xx

   arp -s 191.12.3.77 00:20:4a:xx:xx:xx (Unix)
   arp -s 191.12.3.77 00-20-4a-xx-xx-xx (Windows)

b. Open a Telnet connection to port 1. The connection fails quickly, but the unit temporarily changes its IP address to the one designated in this step.

   telnet 191.12.3.77 1

c. Open a Telnet connection to port 9999, and press Enter within three seconds to go into Setup Mode. If you wait longer than three seconds, the unit reboots and you will have to repeat Step 2.

   telnet 191.12.3.77 9999

d. Select 0 (Server Configuration) and follow the prompts until you get to IP address.

e. Enter the new IP address, subnet mask, and gateway (if applicable).

f. Select 9 to save and exit Setup Mode. The unit performs a power reset.

5-1.3.4 DHCP: The unit ships with a default IP address of 0.0.0.0, which automatically enables DHCP. If a DHCP server exists on the network, it provides the unit with an IP address, gateway address, and subnet mask when the unit boots up.

The DeviceInstaller software can be used to search the network for the DHCP assigned IP address and add it to the list of devices retrieved.

NOTE

This DHCP address does not appear in the unit's Setup Mode or in Web Manager. You can determine your unit's DHCP-assigned IP address in Monitor Mode. When you enter Monitor Mode from the serial port with network connection enabled and issue the NC (Network Communication) command, you see the unit's IP configuration.

5-1.3.5 AutoIP: The unit ships with a default IP address of 0.0.0.0, which automatically enables Auto IP within the unit. AutoIP is an alternative to DHCP that allows hosts to obtain an IP address automatically in smaller networks that may not have a DHCP server. A range of IP addresses (from 169.254.0.1 to 169.254.255.1) has been explicitly reserved for AutoIP-enabled devices. Do not use this range of Auto IP addresses over the Internet.

- If your unit cannot find a DHCP server, and you have not manually assigned an IP address to it, the unit automatically selects an address from the AutoIP reserved range. Then, your unit sends out a (ARP) request to other nodes on the same network to see whether the selected address is being used.
- If the selected address is not in use, then the unit uses it for local subnet communication..
- If another device is using the selected IP address, the unit selects another address from the AutoIP range and reboots. After reboot, the unit sends out another ARP request to see if the selected address is in use, and so on.

AutoIP does not replace DHCP. The unit continues to look for a DHCP server on the network. If it finds a DHCP server, the unit switches to the DHCP server-provided address and reboots.

NOTE

If a DHCP server is found, but it denies the request for an IP address, the unit does not attach to the network, but waits and retries.

AutoIP can be disabled by setting the unit's IP address to 0.0.1.0. This setting enables DHCP but disables AutoIP.

5**-1.3.6 BOOTP:** Similar to DHCP, but for smaller networks. Automatically assigns the IP address for a specific duration of time.

5-1.3.7 Device Server Setup: The Channel Configuration section of the Setup Mode is used to define how the serial port responds to network and serial communications when operating as a device server. See the Xport Users Guide Chapter 7 (Setup Mode: Channel Configuration) section for more details on each of these entries. Some of the important settings in this section are:

Baudrate: This is the baudrate used by the Xport to communicate to the 8210A when in device server mode. This setting must match the rate used by the 8210A, and is typically 9600.

I/F (Interface) Mode: The Interface (I/F) Mode is a bit-coded byte entered in hexadecimal notation. This setting controls the serial port settings of the device server, such as number of bits, parity, stop bits, etc. The default value for this parameter is 4C, which specifies RS-232C, 8-bit, No Parity, 1 stop bit.

Flow: Flow control sets the local handshaking method for stopping serial input/output. The default setting for this parameter is 00 (no flow control)

Port Number: The setting represents the source port number in TCP connections. It is the number that is used to establish a connection via the network interface. The default setting for this parameter is 10001. This number may have to be changed to match the user's software. Certain ports are reserved and should not be used. Refer to the section in the Xport Users Guide for a detailed list.

Compatibility note: units previously mfg'd using the Lantronix MSS-LITE were set to communicate via port 3001

Connect Mode: Connect Mode defines how the unit makes a connection, and how it reacts to incoming connections over the network. Enter Connect Mode options in hexadecimal notation. The default setting is C0, which sets the following options:

Incoming Connection - Always Accept
Response - Nothing (quiet)
Active Startup - No active startup

5-1.3.8 Example Setup Using The Serial Port:

a. Set the rear-panel MODE SELECT switch to CONSOLE position.

b. Open a terminal emulator. Set the PC serial port for 9600N81, no flow control. Serial port cable connections to a PC will require the use of a null-modem cable (DTE to DTE device).

c. To access the Xport SETUP mode, you must enter three lowercase 'x' characters within one second after powering on the unit. The easiest way to enter Setup mode is to hold down the 'x' key, and power up the unit.

d. Response should be::

MAC address 00204AC530DB
Software version V6.6.0.2 (080926) XPTEXE
Press Enter for Setup Mode

e. Pressing the 'Enter' key should display the SETUP mode settings:

NOTE

There is a timeout function built into the SETUP mode. If you do not press the 'Enter' key within 2-3 seconds of the signon message appearing, you will need to turn off the power and start again. If the timeout occurs, you will see the characters "**?!?**" displayed on the screen.

***** basic parameters**
Hardware: Ethernet TPI
IP addr - 0.0.0.0/DHCP/BOOTP/AutoIP, no gateway set
DNS Server not set
DHCP device name : not set

***** Security**
SNMP is enabled
SNMP Community Name: public
Telnet Setup is enabled
TFTP Download is enabled
Port 77FEh is enabled
Web Server is enabled
Web Setup is enabled
ECHO is disabled
Enhanced Password is disabled
Port 77F0h is enabled

***** Channel 1**
Baudrate 9600, I/F Mode 4C, Flow 00
Port 10001
Connect Mode: C0
Send '+++' in Modem Mode enabled
Show IP addr after 'RING' enabled
Auto increment source port disabled
Remote IP Adr: --- none ---, Port 00000
Disconn Mode: 00
Flush Mode: 00

***** Expert**
TCP Keepalive: 45s
ARP cache timeout: 600s
CPU performance: Regular
Monitor Mode @ bootup: enabled
RS485 tx enable: active low
HTTP Port Number: 80
SMTP Port Number: 25
MTU Size: 1400
Alternate MAC: disabled
Ethernet connection type: auto-negotiate

***** E-mail**
Mail server: 0.0.0.0
Unit :
Domain :
Recipient 1:
Recipient 2:

- Trigger 1
Serial trigger input: disabled
Channel: 1
Match: 00,00
Trigger input1: X
Trigger input2: X
Trigger input3: X
Message :
Priority: L
Min. notification interval: 1 s
Re-notification interval : 0 s

- Trigger 2
Serial trigger input: disabled
Channel: 1
Match: 00,00
Trigger input1: X
Trigger input2: X
Trigger input3: X
Message :
Priority: L
Min. notification interval: 1 s
Re-notification interval : 0 s

- Trigger 3
Serial trigger input: disabled
Channel: 1
Match: 00,00
Trigger input1: X
Trigger input2: X
Trigger input3: X
Message :
Priority: L
Min. notification interval: 1 s
Re-notification interval : 0 s

Change Setup:
0 Server
1 Channel 1
3 E-mail
5 Expert
6 Security
7 Defaults
8 Exit without save
9 Save and exit Your choice ?

To change the IP settings of the device server, Select '0' (Server)

At the prompts, enter the desired settings.

For example, to set an IP = 10.100.103.1, netmask = 255.255.255.0, with no gateway:

IP Address : (000) 10.**(000)** 100.**(000)** 103.**(000)** 1
Set Gateway IP Address (N) ?
Netmask: Number of Bits for Host Part (0=default) (0) 8
Set DNS Server IP addr (N) ?
Change telnet config password (N) ?

Change Setup:
0 Server
1 Channel 1
3 E-mail
5 Expert
6 Security
7 Defaults
8 Exit without save
9 Save and exit Your choice ?

Parameters stored ...

Turn off power. To verify the settings you can use the Xport Monitor Mode. To enter Monitor mode, hold down the 'z' key while powering up the unit. After a few seconds, you should see

***** NodeSet 2.0 *****

0>zzzzzzzzzzz

9>

Enter 'NC' in uppercase letters, which is the Network Connection command, whose function is to display the unit's IP configuration

9>NC

IP 010.100.103.049 GW 010.100.103.254 Mask 255.255.255.000 NS 010.100.103.173

0>

NOTE

The parameters shown above were obtained with the Xport set for DHCP mode (IP=0.0.0.0)

Enter 'QU' to quit and exit diagnostics monitor mode.

0> QU

Place the MODE SELECT switch to the ETHERNET position.

To verify network connectivity, you can open a command prompt window on the PC (Start menu | Run… | CMD) and ping the assigned IP address.

C:\WINDOWS>ping 10.100.103.49

Pinging 10.100.103.49 with 32 bytes of data:

Reply from 10.100.103.49: bytes=32 time=7ms TTL=64
Reply from 10.100.103.49: bytes=32 time<1ms TTL=64
Reply from 10.100.103.49: bytes=32 time<1ms TTL=64
Reply from 10.100.103.49: bytes=32 time<1ms TTL=64

Ping statistics for 10.100.103.49:

Packets: Sent = 4, Received = 4, Lost = 0 (0% loss),

Approximate round trip times in milli-seconds:

Minimum = 0ms, Maximum = 7ms, Average = 1ms

You should now be able to communicate with the device. To send commands, you can use the Windows Telnet application to open a connection to Port 10001 (the default serial device tunnel port)

```
C:\WINDOWS>telnet 10.100.103.49 10001
```

Characters that you type in the telnet window will be sent to the device. For example, typing “*IDN?” Should get a response similar to:

```
Weinschel, 8310, 001, V2.98
```

NOTE

By default, the controller does not echo received characters, so the telnet client must be set for 'local echo' in order to see the characters that you type. Optionally, you can send the command “ECHO 1” to set the controller to echo received characters.

5-2. Serial Operation: The serial interface (RS232/RS422) provides a means of remotely programming the 8310 via external computer. The 8311-XXX-X-XN provides for user-selectable communications parameters via a DIP switch (SW1), including baud rate, data format, and handshaking method. LED indicators are provided for transmit (TX) and receive (RX) activity. Selection between RS232/RS422 mode is controlled via an internal 4 position DIP switch SW2, which also provides for user-selectable 120 ohm terminations for the RS422 receiver lines. The RS422 mode transceivers are electrically compatible with RS485.

SW2	RS232	RS422 RS485	Description
1	OFF	User Select	CTS Termination On = Termination Off = No Termination
2	OFF	User Select	RXD Termination On = Termination Off = No Termination
3	OFF	ON	RI/RTS Select
4	ON	OFF	Serial Mode On = RS232 Off = RS422

The data format includes a start bit, eight data bits, and one stop bit (N81). The Baud Rate may be set to 2400, 9600, 19200, or 34800. Parity selections include settings for None, Even, or Odd parity. Handshaking may be enabled, if desired, and the method may be set to either hardware (RTS/CTS) or software (XON/XOFF). For interactive terminal use, echoing may be enabled, in which the 8210A will echo all characters received back to the terminal.

All data and commands are encoded using the ASCII character set. The syntax for commands is the same as for GPIB operation, and uses the syntax structure defined by IEEE 488.2, with the exception of the command termination rules. Commands sent to the 6853may be terminated with either an ASCII CR (0x0D) or ASCII LF (0x0A) character. By default, all responses from the 6853are terminated in an ASCII CR/LF sequence (0x0D followed by 0x0A).

Software handshaking uses the XON/XOFF scheme in which an ASCII DC3 (0x13) character is transmitted by the receiver to indicate that data transmission should be halted (XOFF), and an ASCII DC1 (0x11) character is transmitted to indicate that data transmission may continue (XON). Hardware handshaking utilizes the RTS and CTS lines. When the RTS output signal is asserted true, the unit is ready for data. This signal should be connected to the external computer's CTS input signal, so that when the receiver is ready, the transmitter may send data. When the unit is not ready for data, it unasserts the RTS signal, halting data transmission. Likewise, the unit monitors the CTS input signal during data transmission, halting transmission if the external computer unasserts it's RTS signal. In addition, the 6853unasserts the RTS signal while command execution is in progress.

For those systems incorporating local front panel controls, the serial port can lockout local users, providing a Remote/ Local function similar to that of GPIB operation.

5-5.1. RS-232 Operation: The RS-232 Serial port is a 9-pin connector that is compatible with the pin-out of the serial port on a PC. It allows the use of a null-modem style cable. The pin-out for the connector is show below. For clarity, the signal names and directions are relative to the 6631.

Pin	Signal Name	Description	Direction
1	DCD	unused	---
2	RxD	Receive data	input
3	TxD	Transmit data	output
4	DTR	Signals DTE is on-line	output
5	GND	Ground	---
6	DSR	unused	---
7	RTS	Signals DTE is ready	output
8	CTS	Signals DCE is ready	input
9	RI	unused	---

The DTR signal is asserted when power is on, indicating that the unit is ready.

RS232
9-pin DB9
Pinout

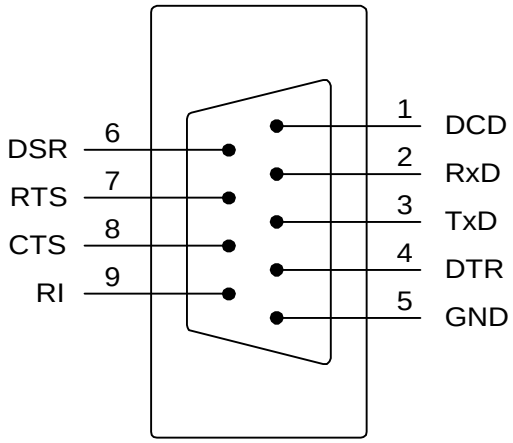

Null Modem Cable

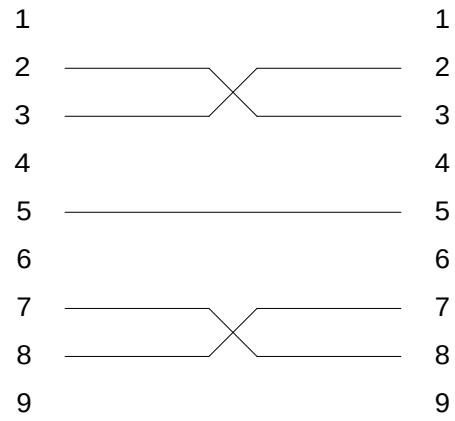

5-3. Status Reporting

The 6853 implements the 488.2 Status Reporting Structure, which utilizes the IEEE488.1 status byte with additional data structures and rules. The Status Byte Register can be read with either a serial poll (IEEE-488 operation only) or the *STB? common query command. The Service Request Enable Register (SRE) allows the user to select which bits in the Status Byte Register may cause service requests. A bit value of one indicates that the corresponding event is enabled, while a bit value of zero disables an event. The Service Request Enable Register may be accessed with the *SRE and *SRE? common commands. The Status Byte Register may be cleared with the *CLS common command, with the exception of the MAV bit, which is controlled by the operation of the Output Queue. The SRE Register is set to 0 at power-on, disabling all events.

Status Byte Register/ Service Request Enable Register Formats

D7	D6	D5	D4	D3	D2	D1	D0
	RQS	ESB	MAV		EEQ		

Bit	Mnemonic	Description
6	RQS	Request Service: This bit, if set, indicates that the device is asserting the SRQ signal.
5	ESB	Event Status Bit: This bit is true when an enabled event in the Event Status Register is true.
4	MAV	Message Available: This bit is true when there is valid data available in the output queue.
2	EEQ	Error/Event Queue: This bit is true when there is Error/Event data available in the Error/Event queue.

The Standard Event Status Register is used to report various IEEE 488.2-defined events. The register contents may be accessed with the *ESR? command. An Event Status Enable Register allows the user to select which bits in the ESR that will be reflected in the ESB summary message bit of the Status Byte Register. The Event Status Enable Register may be accessed with the *ESE and *ESE? common commands. The Event Status Register is cleared by an *ESR? query or *CLS common command. The ESE Register is set to 0 at power-on, disabling all events.

Standard Event Status Register/ Standard Event Status Enable Register Formats

D7	D6	D5	D4	D3	D2	D1	D0
ON	URQ	CME	EXE	DDE	QYE	RQC	OPC

Bit	Mnemonic	Description
7	PON	Power On: This bit indicates that the device has powered-on
6	URQ	User Request: This event bit indicates that a local control is causing a User Request
5	CME	Command Error: The parser has detected a syntax error in the current command.
4	EXE	Execution Error: The command could not be properly executed due to an illegal input range or other inconsistent data.
3	DDE	Device Dependent Error: A command could not properly complete due to some device specific error
2	QYE	Query Error: This bit indicates that either an attempt has been made to read data when there was none present, or that data in the Output Queue has been lost
1	RQC	Request Control: The device is requesting control (not implemented)
0	OPC	Operation Complete: This bit is generated in response to an *OPC command. It indicates that the ITS 2000 has completed all pending operations.

The Status Reporting Registers may be used for serial communications, with certain limitations. The Status Byte Register can only be read via the *STB? query command, as the comm port does not provide for a serial poll operation. Also, as data in the Output Queue is sent automatically during serial operation, the MAV message available bit in the STB serves no purpose.

5-4. GENERAL SYNTAX STRUCTURE: The following paragraphs outline the general syntax and command structure for the Model 6631. This structure is common to all bus flavors of the Model 6631.

NOTE

In the descriptions that follow, the term whitespace is used to define a sequence of one or more combinations of ASCII Space (20h), Carriage return (0Dh), or Tab (09h) characters.

5-4.1 SYNTAX OF QUERIES: A query message unit is made up of a query header ending in an ASCII question mark character '?' (3FH), followed by optional whitespace, and ended by a program message terminator. To form a multiple query, separate the individual program message units with a semicolon.

Examples : "ATTN?"
"ASSIGN?"

b. Multiple Query Commands:

"ATTN?; ASSIGN?"

5-4.2 SYNTAX OF COMMANDS: A command message unit is made up of a command header, optionally followed by an argument and units, and ended by a program message terminator. If multiple commands are made on the same program line, separate the individual command messages with a semicolon.

Arguments - The 6853supports a variety of argument types that can be used in program commands. These types are:

- Character Program Data
- Integer Numeric Program Data
- Real Numeric Program Data

Each data type has its own rules of syntax. The following paragraphs provide the syntax rules for each of the argument types listed above.

Character Program Data-This data type is comprised of the set of printable ASCII characters (excluding those used as delimiters). Character program data represents alpha or alphanumeric strings. The use of alpha characters is case-insensitive. If the first character of the string is not an alpha character, then the string must be delimited with either the ASCII single-quote (') or double-quote (") character in order to distinguish the string from a numeric data type.

Examples: ATTEN1
ON
"150T"

Integer Numeric Program Data-This data type is used to represent integer, binary, or hexidecimal numeric information, all of which may be used interchangeably. Integer data is comprised of the numeric digits '0'-'9', binary data is comprised of the digits '0' and '1' preceded by the characters '#B', and hexidecimal data is comprised of the digits '0'-'9', and the letters 'A'-'F', preceded by the characters '#H' or the C language style prefix '0x'.

Examples: 123 (integer)
#H55 (hex)
0xAA (hex)
#B1010 (binary)

Real Numeric Program Data-This data type includes decimal numbers containing a sign, decimal point, and/or an exponent. The format is as follows: [sign]digits[.[digits][E[sign]digits]]

Examples: 2
2.5
-35.25E+2

In the command descriptions that follow, argument types are also described using the following additional conventions to indicate the relative size of the parameter:

byte	- used to indicate an 8-bit unsigned integer
word	- used to indicate a 16-bit unsigned integer
int8	- 8-bit integer
int16	- 16-bit integer
int32	- 32-bit integer
string	- character data, including the max number of characters allowable. (i.e., string8 has a max of 8 chars)

5-4.3 OUTPUT DATA FORMAT: Output data from the Model 6853 consists of a series of ASCII digits and message strings, terminated with an ASCII Line-Feed character (0AH), in response to a program message that contains one or more query commands. In the case of multiple query commands in the same program message, the data resulting from each of the individual message units will be separated by an ASCII comma (2CH) character.

5-4.4 NOTATIONAL CONVENTION.

[ ] Brackets indicate optional arguments or parameters.

{ } One and only one of the enclosed entries must be selected unless the field is also surrounded by brackets, in which case it is optional.

... Ellipses indicate that the preceding argument or parameter may be repeated.

[,...] The preceding item may be repeated, but each repetition must be separated by a comma.

5-5. COMMON COMMANDS

***CLS**
Function: Clears the Status Byte and Event Status Registers.
Syntax: *CLS
Argument(s): none
Remarks: This function is used to clear the Status Byte and the Event Status Registers.
Return Value: none
Example(s): *CLS

***ESE**
Function: Sets the Event Status Enable Register.
Syntax: *ESE *mask*
Argument(s): *mask* integer bitmask
Remarks: This function is used to set the Event Status Enable Register to the value specified by mask.
Return Value: none
Example(s): *ESE 255

***ESE?**
Function: Reads the Event Status Enable Register.
Syntax: *ESE?
Argument(s): none
Remarks: This function is used to read the Event Status Enable Register.
Return Value: *mask* integer register mask
Example(s): *ESE? returns the following '255'

***ESR?**
Function: Reads the Event Status Register
Syntax: *ESR?
Argument(s): none
Remarks: This function is used to read the Event Status Register. Reading the register clears it.
Return Value: *reg* integer register
Example(s): *ESR? returns the following '128'

***SRE**
Function: Sets the Status Byte Enable Register
Syntax: *SRE *mask*
Argument(s): *mask* integer bitmask
Remarks: This function is used to set the Status Byte Enable Register to the value specified by *mask*.
Return Value: none
Example(s): *SRE 255

***SRE?**
Function: Reads the Status Byte Enable Register.
Syntax: *SRE?
Argument(s): none
Remarks: This function is used to read the Status Byte Enable Register.
Return Value: *mask* integer register mask
Example(s): *SRE? returns the following '255'

***STB?**
Function: Reads the Status Byte Register.
Syntax: *STB?
Argument(s): none
Remarks: This function is used to read the Status Byte Register.
Return Value: *reg* integer register
Example(s): *STB? returns the following '96'

***IDN?**
Function: Reads the system identification information.
Syntax: *IDN?
Argument(s): none
Remarks: This function is used to read the system identification information, which is a string consisting of the following data: manufacturer, model, serial number, and firmware version.
Return Value: *mfg* integer count of devices
Example(s): *IDN? returns the following 'Weinschel,8311 Series, 123, 1.00A'

***RST**	**Function:**	Performs a device reset.
	Syntax:	*RST
	Argument(s):	none
	Remarks:	This function is used to reset the device.
	Return Value:	none
	Example(s):	*RST
***OPC**	**Function:**	Operation complete service request.
	Syntax:	*OPC
	Argument(s):	none
	Remarks:	This function generates the Operation Complete message (OPC) in the Standard Event Status Register when all pending device operations have finished.
	Return Value:	none
	Example(s):	*OPC
***OPC?**	**Function:**	Operation complete query
	Syntax:	*OPC?
	Argument(s):	none
	Remarks:	This function loads a '1' into the output queue when the Program Message Unit is executed. Its primary use is to provide an indication of command completion by including the command as the last one in a series of commands.
	Return Value:	1 integer command completed
	Example(s):	SAVE ASSIGN; *OPC? returns a '1' when the SAVE ASSIGN command completes.
***WAI**	**Function:**	Wait To Continue
	Syntax:	*WAI
	Argument(s):	none
	Remarks:	This function prevents the8311 Series from executing any further commands or queries until there are no pending operations. The 8311 Series executes all commands sequentially, and does not allow overlapping commands.
	Return Value:	none
	Example(s):	*WAI

5-6. GENERAL COMMANDS:

CHAN	**Function:**	Selects the currently active channel
	Syntax:	CHAN *chnum*
	Argument(s):	*chnum* integer channel number
	Remarks:	This function is used to select the currently active channel.
	Return Value:	none
	Example(s):	CHAN 1
CHAN?	**Function:**	Reads the current channel number
	Syntax:	CHAN?
	Argument(s):	none
	Remarks:	This function is used to read the currently active channel number.
	Return Value:	*chnum* integer current channel number
	Example(s):	CHAN? returns '1'
ATTN	**Function:**	Set attenuation
	Syntax:	ATTN *atten*
	Argument(s):	atten real desired value, in dB
	Remarks:	This function sets the attenuation of the currently selected channel to atten.
	Return Value:	none
	Example(s):	ATTN 63 ATTN 12.25 ATTN 45.0
ATTN?	**Function:**	Read attenuation
	Syntax:	ATTN?
	Argument(s):	none
	Remarks:	This function reads the attenuation of the currently selected channel.
	Return Value:	*atten* real attenuation value, in dB
	Example(s):	ATTN? returns '63.00'
REL	**Function:**	Sets relative display mode for the current channel
	Syntax:	REL *mode*
	Argument(s):	*mode* integer relative mode on/off
	Remarks:	This function is used to set the relative display mode of operation for the current channel. A value of 0 for the parameter mode will turn relative mode off, while a value of 1 will turn relative mode on.
	Return Value:	none
	Example(s):	REL 1
REF	**Function:**	Sets reference
	Syntax:	REF
	Argument(s):	none
	Remarks:	This function sets the reference value for the active channel to the current attenuation setting. This command is used for the REL and RELATTN functions.
	Return Value:	none
	Example(s):	REF; REL 1 sets the reference, and turns on relative mode
REF?	**Function:**	Read reference setting
	Syntax:	REF?
	Argument(s):	none
	Remarks:	This function reads the reference setting of the currently selected channel.
	Return Value:	*refatten* real reference attenuation value, in dB
	Example(s):	REF? returns '30.00'

RELATTN	**Function:**	Sets attenuation relative to the reference setting
	Syntax:	RELATTN atten
	Argument(s):	*atten* real desired value, in dB
	Remarks:	This function sets the attenuation of the currently selected channel to atten, relative to the reference value set when the REL command was executed.
	Return Value:	none
	Example(s):	RELATTN 10 increases the attenuation setting 10dB from the reference setting RELATTN -10 decreases the attenuation setting by 10dB from the reference setting 15.
RELATTN?	**Function:**	Read relative attenuation of the current channel
	Syntax:	RELATTN?
	Argument(s):	none
	Remarks:	This function reads the relative attenuation of the currently selected channel.
	Return Value:	*relatten* real relative attenuation value, in dB
	Example(s):	RELATTN? returns '-10.00'
STEPSIZE	**Function:**	Sets attenuation stepsize for the current channel
	Syntax:	STEPSIZE atten
	Argument(s):	*atten* real desired stepsize value, in dB
	Remarks:	This function sets the attenuation stepsize for the INCR and DECR commands for the current channel to atten. The default value of the attenuator's stepsize is the intrinsic resolution of the attenuator, i.e., a 127dB/1dB step attenuator has a default stepsize of 1dB.
	Return Value:	none
	Example(s):	STEPSIZE 10 changes the stepsize to 10dB
STEPSIZE?	**Function:**	Read attenuation stepsize
	Syntax:	STEPSIZE?
	Argument(s):	none
	Remarks:	This function reads the attenuation stepsize of the current channel.
	Return Value:	*atten* real attenuation stepsize value, in dB
	Example(s):	STEPSIZE? returns '10.00'
INCR	**Function:**	Increments attenuation
	Syntax:	INCR
	Argument(s):	none
	Remarks:	This function increments the attenuation setting of the current channel by the value of the attenuator's programmed stepsize (see STEPSIZE command).
	Return Value:	none
	Example(s):	INCR
DECR	**Function:**	Decrements attenuation
	Syntax:	INCR
	Argument(s):	none
	Remarks:	This function decrements the attenuation setting of the current channel by the value of the attenuator's programmed stepsize (see STEPSIZE command).
	Return Value:	none
	Ex	

6. MAINTENANCE:

The following paragraphs provide general inspection and maintenance guide-lines for the Model 8310-XXX-XN Attenuator Unit.

6-1. INSPECTION: Perform a visual inspection in conjunction with the maintenance activities schedule when a malfunction is suspected, or whenever an assembly is removed or replaced.

6-2. PREVENTIVE MAINTENANCE: While the 8310 requires very little preventive maintenance, it should not be subjected to physical abuse, severe mechanical shock, high humidity, or operating temperatures outside the specification range. The instrument should be kept free of excessive dirt and dust, since these can interfere with connector functions and with normal heat dissipation. For cleaning instructions refer to paragraph 6-3 (special cleaning instructions). The following paragraphs provide the preventive maintenance that is to be performed on the Unit.

Care should be taken to prevent strain on the interconnecting cables, since damage here may not always be apparent. Occasionally check the external cables and connectors for signs of cracked insulation and/or bent or worn pins. Tests show that connectors must be clean for accuracy and stability. This requires an inspection and cleaning of each connector immediately before use. For connector cleaning instructions, refer to paragraph 6-3. When cleaning precautions are observed regularly, connectors can maintain their stability for over several thousand connection cycles. Refer to Appendix A for more information about cables and connectors.

6-3. SPECIAL CLEANING INSTRUCTIONS: The cleaning procedures for 8310 are divided into five general groups: microwave coaxial cable assemblies, circuit card and modules; machined surfaces and hardware, chassis cleaning, and connector cleaning.

6-3.1. MICROWAVE COAXIAL CABLE ASSEMBLIES: Appendix A (located at the end of this manual) provides all the necessary procedures for care, cleaning, and handling of microwave coaxial cable assemblies.

6-3.2 CIRCUIT CARDS AND MODULES: A protective coating is applied to circuit cards for protection from moisture, arcing, short-circuiting, and abrasion. To remove light dirt from circuit cards and modules proceed as follows:

CAUTION

- DO NOT use a nylon bristle brush in the solvent as the bristles may dissolve and cause damage to the circuit card or component.
- DO NOT use ultrasonic cleaning on parts or assemblies containing electrical or electronic components.
- DO NOT bend pins of electrical connectors when using fiber-bristle brush.

a. Briskly brush isopropyl alcohol onto area to be cleaned with fiber-bristle brush.

b. Carefully remove residue with a clean lint-free cloth and repeat step "a" as a rinse.

WARNING

Compressed air used for cleaning and/or drying can create airborne particles that may enter the eye. Goggles/ faceshields should be worn. DO NOT direct air stream towards self or other personnel. Pressure should be restricted to a maximum 15 psi to avoid personal injury.

c. When parts are thoroughly clean, dry parts using 5 psi of clean moisture free compressed air or preferably dry nitrogen (pressurized spray will work well).

6-3.3 MACHINED SURFACES AND HARDWARE: To remove light dirt and dust from mechanical parts such as castings, covers and other hardware proceed as follows:

WARNING

Compressed air used for cleaning and/or drying can create airborne particles that may enter the eye. Goggles/ face-shields should be worn. DO NOT direct air stream towards self or other personnel. Pressure should be restricted to a maximum 15 psi to avoid personal injury.

CAUTION

- Under no circumstances use a wire brush, steel wool, or abrasive compound. Using these items will cause extensive damage to the instrument's surface.
- DO NOT use a nylon bristle brush in solvent as the bristles may dissolve and cause damage to the circuit card or component.

a. Use 5 psi of clean, moisture-free compressed air or preferably dry nitrogen to blow loose dirt and dust from surface of item.

b. Briskly brush isopropyl alcohol onto area to be cleaned with a fiber-bristle brush.

c. Remove residue with lint-free cloth and repeat step "b" as a rinse.

d. When parts are thoroughly clean, dry parts using 5 psi of clean, moisture-free compressed air or preferably dry nitrogen.

e. Clean smaller mechanical parts or hardware by dipping into a container of isopropyl alcohol. Remove dirt by brushing with fiber-bristle brush after parts have been immersed for several hours.

f. Remove parts from isopropyl alcohol and rinse by immersing into a different container of isopropyl alcohol.

g. When parts are thoroughly cleaned, dry parts using 5 psi of clean, moisture-free compressed air or preferably dry nitrogen.

6-3.4 CHASSIS CLEANING: Clean chassis using a lint-free cloth moistened with water and mild detergent. For harder to clean areas, such as inside corners of chassis, use a vacuum cleaner.

6-3.5 CONNECTOR CLEANING: Where small amounts of rust, corrosion, and/or oxide deposits are present on connectors, clean externally with a soft-bristle brush, aluminum wool, or internally with an acid brush; then wash with a non-corrosive solvent. MIL-C-83112 is recommended. Exercise care to ensure no metal filing or residue remains inside the connector and the connector is thoroughly dry. Where rust, corrosion, and/or oxide deposits are present in large quantities, replace the connector.

6-4. LINE VOLTAGE FUSE REPLACEMENT: The following steps provide procedures to replace the line voltage Fuse Assembly. This unit accepts a F1.5A, 250 Vac fuse for 115 Vac.

WARNING

Sufficient power levels are present at the Power Input Assembly to cause personal injury. Ensure that the instrument power cord is DISCONNECTED before attempting to change fuses.

CAUTION

DO NOT connect or apply power to this instrument until the Power Entry Module Assembly has been adjusted to the operational line voltage.

a. Disconnect the power cord from the Power Entry Module Assembly.

b. Use a small screwdriver to carefully open the Fuse Drawer.

c. Slide out Fuse Drawer located in the center of the Power Entry Module Assembly.

d. Remove defective fuse and replace with the correct fuse (Refer to applicable parts list for fuse part number).

e. Snap the Fuse Drawer shut and re-connect ac power cord.

7. REPLACEABLE PARTS LIST:

This section lists and describes the parts located in the Model 8310-XXX-XN Programmable Attenuator Units (P/N 193-730X-X). The Replaceable Parts Lists (RPL) is intended for use in identifying, locating, and requisitioning assemblies and components for the Model 8310-XXX-XN.

7-1 UNDERSTANDING REFERENCE DESIGNATORS: All assemblies and electrical parts are identified by standard reference designators (resistors R1, for example). Reference designators are used in parts lists and on parts identification drawings. The title of a parts list or drawing contains the reference designator or the assembly or subassembly to which it applies. The designators in the parts list, as a prefix, but omitted from the list to make it easier to locate a specific part. To complete a reference designator in a parts list, precede the designator for the specific part (DS1, for example) with the designator in the title (A6, for example) to form a complete reference designator for the part (in this case, A6DS1).

7-2 ORDERING INFORMATION: When ordering parts from Aeroflex / Weinschel, please include the following information:

- Aeroflex / Weinschel part number.
- Description of the component or part.
- Model and serial number of the instrument.
- Assembly number and assembly revision (if any) from the assembly (this information is on the component side of the PCB).

7-3 DRAWING NUMBER: The Aeroflex / Weinschel part number consists of a basic number with a dash number. The basic number should cross reference to a drawing number for most of the items. For those items that do not have a drawing number, the manufacturers part number is provided.

7-4 REPLACEABLE PARTS LIST (RPL): This RPL contains a breakdown of the instrument into its major assemblies and detailed parts. The following paragraphs describe the contents of each column of the RPL.

7-4.1 REFERENCE DESIGNATOR: This column contains reference designations arranged in alphanumerical sequence. The letters A thru Z have precedence, followed by numerals 0 thru 9. In addition to the reference designators that are listed, some mechanical parts are also listed. These items lack reference designators and are included because they are considered subject to wear and/or breakage, or because they are custom (non-standard) hardware or parts that might become lost or damaged. This column contains the word N/A for those items or parts not having a reference designator.

7-4.2 DESCRIPTION: This column contains the nomenclature located in the title block of the engineering drawing by the designing activity. The noun name is listed first, followed by modifiers and descriptive information to completely identify the part or assembly.

7-4.3 PART NUMBER: This column contains the Aeroflex / Weinschel part number assigned to an assembly, sub-assembly, or detailed part. This also includes Aeroflex / Weinschel numbers for specification control, source control, and altered items drawings.

7-4.4 VENDOR PART NO.: This column contains manufacturers part numbers for those parts Aeroflex / Weinschel purchases as off the shelf items and assigns Aeroflex / Weinschel part numbers for internal control only. These parts may be ordered through the manufacturer or through Aeroflex / Weinschel by the Aeroflex / Weinschel part number.

7-4.5 CAGE CODE: This column provides the Commercial and Government Entity (CAGE) code on the same line as the applicable part number. Codes, names, and addresses of venders with an assigned CAGE are listed in Cataloging Handbook H4-1 and H4-2. Vendors that have not been assigned CAGE codes by the government are identified by the word NONE in this column. The names and addresses of these venders can be obtained from Aeroflex / Weinschel. Part numbers that have no CAGE numbers listed are manufactured or altered by Weinschel.

7-4.6 ASSEMBLY AND COMPONENT LOCATION: The assembly/component location and schematic diagrams for the different 8310-XXX-XN series models are located in rear of this manual by the drawing number. Drawing find numbers have also been included to help locate components or hardware.

Model 8310-38-FN, Attenuator Unit Assembly Replaceable Parts List (P/N 193-7302-3, Rev. B):

Find No.	Part Number	Description	Quantity Used	Reference Designator	CAGE Code	Vendor Part Number
1	193-8138-1	ASSY, ATTEN, BASE UNIT, Model 8311 W/ETHERNET (+15V)	1	NA		
2	193-8039	MOUNTING PLATE	2	NA		
3	3206T-1	ATTEN PRGM W/SMARTSTEP INTER	6	AT1 - AT6		
4	074-912	KIT, RACK MOUNTING W/O HANDLES 3.5 H	1	NA	24803	K2RMX-001A
5	193-8096-1	OVERLAY, REAR PANEL	1	NA		
6	068-32-6/0	COAXIAL CABLE ASSY, SMA M/ TYPE N FEMALE, CONFORMABLE, DC-11 GHz	6	W8, W10, W12, W14, W16, W18	93459	068-50-6/0
7	193-8049	OVERLAY, PANEL BLANK	1	NA		
8	193-11347	SPACER, CONN, 12 POS	1	NA		
9	063-408	N -TYPE, CONNECTOR	12	NA		
10	193-8116	ASSY, CABLE, CNTRL TO ATTEN (6 ATTEN)	1	W7		
11	MS24693-C3	SCR FLAT HD 4-40 X 5/16 LG 100	12	NA		
13	NAS1635-04LR4	SCR PAN HD SELFLOCK, 4-40 X 1/4	12	NA		
15	090-445	* LABEL, REFERENCE INSTRUCTION MANUAL	1	NA		
16	090-354	* LABEL WARNING, HIGH VOLTAGE	1	NA		
17	074-889-4	LABEL, THERMAL TRANSFER, PERM MTLZ, POLTEST, 1.50 X .75IN	1	NA	BRADY	THT-6-428-10
20	068-32-13/0	COAXIAL CABLE ASSY, SMA M/ TYPE N FEMALE, CONFORMABLE, DC-11 GHz	6	W9, W11, W13, W15, W17, W19		
22	089-4157	ICD, ATTEN UNIT, 8311-38-X-N	0	NA		
23	193-8150	WIRING DIAGRAM, 8311-38-X-N	0	NA		
24	IM501	O & S, ATTEN UNIT, MODEL 8311 (+15V) W/ETHERNET	1	NA		

Refer to Aeroflex / Weinschel Drawing 193-7302-3, Rev. B for parts location.

Model 8310-38-RN, Attenuator Unit Assembly Replaceable Parts List (P/N 193-7302-4, Rev. B):

Find No.	Part Number	Description	Quantity Used	Reference Designator	CAGE Code	Vendor Part Number
1	193-8138-1	ASSY, ATTEN, BASE UNIT, Model 8311 W/ETHERNET (+15V)	1	NA		
2	193-8039	MOUNTING PLATE	2	NA		
3	3206T-1	ATTEN PRGM W/SMARTSTEP INTER	6	AT1 - AT6		
4	074-912	KIT, RACK MOUNTING W/O HANDLES 3.5 H	1	NA	24803	K2RMX-001A
5	193-8096-1	OVERLAY, REAR PANEL	1	NA		
6	068-32-6/0	COAXIAL CABLE ASSY, SMA M/ TYPE N FEMALE, CONFORMABLE, DC-11 GHz	6	W8, W10, W12, W14, W16, W18	93459	068-50-6/0
7	193-8049	OVERLAY, PANEL BLANK	1	NA		
8	193-11347	SPACER, CONN, 12 POS	1	NA		
9	063-408	N -TYPE, CONNECTOR	12	NA		
10	193-8116	ASSY, CABLE, CNTRL TO ATTEN (6 ATTEN)	1	W7		
11	MS24693-C3	SCR FLAT HD 4-40 X 5/16 LG 100	12	NA		
13	NAS1635-04LR4	SCR PAN HD SELFLOCK, 4-40 X 1/4	12	NA		
15	090-445	* LABEL, REFERENCE INSTRUCTION MANUAL	1	NA		
16	090-354	* LABEL WARNING, HIGH VOLTAGE	1	NA		
17	074-889-4	LABEL, THERMAL TRANSFER, PERM MTLZ, POLTEST, 1.50 X .75IN	1	NA	BRADY	THT-6-428-10
20	068-32-13/0	COAXIAL CABLE ASSY, SMA M/ TYPE N FEMALE, CONFORMABLE, DC-11 GHz	6	W9, W11, W13, W15, W17, W19		
22	089-4157	ICD, ATTEN UNIT, 8311-38-X-N	0	NA		
23	193-8150	WIRING DIAGRAM, 8311-38-X-N	0	NA		
24	IM501	O & S, ATTEN UNIT, MODEL 8311 (+15V) W/ETHERNET	1	NA		

Refer to Aeroflex / Weinschel Drawing 193-7302-4, Rev. B for parts location.

Model 8310-38-R-EN, Attenuator Unit Assembly Replaceable Parts List (P/N 193-7302-13, Rev. B):

Find No.	Part Number	Description	Quantity Used	Reference Designator	CAGE Code	Vendor Part Number
1	193-8138-1	ASSY, ATTEN, BASE UNIT, Model 8311 W/ETHERNET (+15V)	1	NA		
2	193-8039	MOUNTING PLATE	2	NA		
3	3206T-1E	ATTEN PRGM W/SMARTSTEP INTER	6	AT1 - AT6		
4	074-912	KIT, RACK MOUNTING W/O HANDLES 3.5 H	1	NA	24803	K2RMX-001A
5	193-8096-1	OVERLAY, REAR PANEL	1	NA		
6	068-32-6/0	COAXIAL CABLE ASSY, SMA M/ TYPE N FEMALE, CONFORMABLE, DC-11 GHz	6	W8, W10, W12, W14, W16, W18	93459	068-50-6/0
7	193-8049	OVERLAY, PANEL BLANK	1	NA		
8	193-11347	SPACER, CONN, 12 POS	1	NA		
9	063-408	N -TYPE, CONNECTOR	12	NA		
10	193-8116	ASSY, CABLE, CNTRL TO ATTEN (6 ATTEN)	1	W7		
11	MS24693-C3	SCR FLAT HD 4-40 X 5/16 LG 100	12	NA		
13	NAS1635-04LR4	SCR PAN HD SELFLOCK, 4-40 X 1/4	12	NA		
15	090-445	* LABEL, REFERENCE INSTRUCTION MANUAL	1	NA		
16	090-354	* LABEL WARNING, HIGH VOLTAGE	1	NA		
17	074-889-4	LABEL, THERMAL TRANSFER, PERM MTLZ, POLTEST, 1.50 X .75IN	1	NA	BRADY	THT-6-428-10
20	068-32-13/0	COAXIAL CABLE ASSY, SMA M/ TYPE N FEMALE, CONFORMABLE, DC-11 GHz	6	W9, W11, W13, W15, W17, W19		
22	089-4157	ICD, ATTEN UNIT, 8311-38-X-N	0	NA		
23	193-8150	WIRING DIAGRAM, 8311-38-X-N	0	NA		
24	IM501	O & S, ATTEN UNIT, MODEL 8311 (+15V) W/ETHERNET	1	NA		

Refer to Aeroflex / Weinschel Drawing 193-7302-13, Rev B for parts location.

Model 8310-202-2-FN, Attenuator Unit Assembly Replaceable Parts List (P/N 193-7305-4, Rev. A):

Find No.	Part Number	Description	Quantity Used	Reference Designator	CAGE Code	Vendor Part Number
1	193-8138-1	ASSY, ATTEN, BASE UNIT, MODEL 8311 W/ETHERNET (+15V)	1	NA		
2	193-8054	OVERLAY, FRONT PANEL SMA	1	NA		
3	193-8049	OVERLAY, PANEL BLANK	1	NA		
4	193-8042	MOUNTING PLATE	2	NA		
5	193-8118	MOUNTING PLATE	1	NA		
6	150T-11	ATTEN PRGM SMARTSTEP	2	AT2, AT4		
7	150T-110	ATTEN PRGM SMARTSTEP	2	AT1, AT3		
10	1568	ADAPT WPM 3 BULKHD	4	NA		
11	068-32-4/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	2	W9, W12		B068-32-4/0
12	068-32-6/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	2	W8, W10		B068-32-6/0
13	068-32-12/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	2	W11, W13	93459	B068-32-12/0
14	193-9646	CONNECTOR ADAPTER PLATE	6	NA		
15	193-8101-1	ASSY CONTROLLER TO ATTEN	1	W7		
16	074-912	KIT, RACK MOUNTING W/O HANDLES 3.5 H	1	NA	24803	K2RMX-001A
17	074-761-1	HOLE PLUG 3/8 HOLE NYLON BLACK	8	NA	83330	3091
18	074-921	FEET NON-SKID	4	NA	4963	SJ-5008 BLACK
					4963	SJ-5008SP
					24803	KFT12-BLK
19	NAS1635-04LR4	SCR PAN HD SELFLOCK 4-40 X 1/4	12	NA		
20	MS24693-C3	SCR FLAT HD 4-40 X 5/16 LG 100	8	NA		
21	090-354	* LABEL WARNING HIGH VOLTAGE	1	NA		
22	090-445	* LABEL, REFERENCE INSTR MANUAL	1	NA		
25	090-301	* LABEL STD 1.5 X .75 IN	1	NA		
26	IM501	O & S, ATTEN UNIT MODEL 8311 (+15V) W/ETHERNET	1	NA		
27	193-8148	WIRING DIAGRAM MODEL 8311-202-X-XN	0	NA		
28	089-4090	ICD, ATTEN UNIT, MODEL 8311 W/ETHERNET 150 ATTENS	0	NA		

Refer to Aeroflex / Weinschel Drawing 193-7305-4, Rev. A for parts location.

Model 8310-202-3-FN, Attenuator Unit Assembly Replaceable Parts List (P/N 193-7305-5, Rev. A):

Find No.	Part Number	Description	Quantity Used	Reference Designator	CAGE Code	Vendor Part Number
1	193-8138-1	ASSY, ATTEN, BASE UNIT, MODEL 8311 W/ETHERNET (+15V)	1	NA		
2	193-8054	OVERLAY, FRONT PANEL SMA	1	NA		
3	193-8049	OVERLAY, PANEL BLANK	1	NA		
4	193-8042	MOUNTING PLATE	2	NA		
5	193-8118	MOUNTING PLATE	1	NA		
6	150T-11	ATTEN PRGM SMARTSTEP	3	AT2, AT4, AT6		
7	150T-110	ATTEN PRGM SMARTSTEP	3	AT1, AT3, AT5		
10	1568	ADAPT WPM 3 BULKHD	6	NA		
11	068-32-4/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	3	W9, W12, W15		B068-32-4/0
12	068-32-6/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	2	W8,W10		B068-32-6/0
13	068-32-12/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	4	W11, W13, W14, W16	93459	B068-32-12/0
14	193-9646	CONNECTOR ADAPTER PLATE	6	NA		
15	193-8101-1	ASSY CONTROLLER TO ATTEN	1	W7		
16	074-912	KIT, RACK MOUNTING W/O HANDLES 3.5 H	1	NA	24803	K2RMX-001A
17	074-761-1	HOLE PLUG 3/8 HOLE NYLON BLACK	6	NA	83330	3091
18	074-921	FEET NON-SKID	4	NA	4963	SJ-5008 BLACK
					4963	SJ-5008SP
					24803	KFT12-BLK
19	NAS1635-04LR4	SCR PAN HD SELFLOCK 4-40 X 1/4	17	NA		
20	MS24693-C3	SCR FLAT HD 4-40 X 5/16 LG 100	12	NA		
21	090-354	* LABEL WARNING HIGH VOLTAGE	1	NA		
22	090-445	* LABEL, REFERENCE INSTR MANUAL	1	NA		
25	090-301	* LABEL STD 1.5 X .75 IN	1	NA		
26	IM501	O & S, ATTEN UNIT MODEL 8311 (+15V) W/ETHERNET	1	NA		
27	193-8148	WIRING DIAGRAM MODEL 8311-202-X-XN	0	NA		
28	089-4090	ICD, ATTEN UNIT, MODEL 8311 W/ETHERNET 150 ATTENS	0	NA		

Refer to Aeroflex / Weinschel Drawing 193-7307-5, Rev. A for parts location.

Model 8310-202-2-RN, Attenuator Unit Assembly Replaceable Parts List (P/N 193-7305-6, Rev. A):

Find No.	Part Number	Description	Quantity Used	Reference Designator	CAGE Code	Vendor Part Number
1	193-8138-1	ASSY, ATTEN, BASE UNIT, MODEL 8311 W/ETHERNET (+15V)	1	NA		
2	193-8054	OVERLAY, FRONT PANEL SMA	1	NA		
3	193-8049	OVERLAY, PANEL BLANK	1	NA		
4	193-8042	MOUNTING PLATE	2	NA		
5	193-8118	MOUNTING PLATE	1	NA		
6	150T-11	ATTEN PRGM SMARTSTEP	2	AT2, AT4		
7	150T-110	ATTEN PRGM SMARTSTEP	2	AT1, AT3		
10	1568	ADAPT WPM 3 BULKHD	4	NA		
11	068-32-4/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	2	W9, W12		B068-32-4/0
12	068-32-6/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	2	W8, W10		B068-32-6/0
13	068-32-12/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	2	W11, W13	93459	B068-32-12/0
14	193-9646	CONNECTOR ADAPTER PLATE	6	NA		
15	193-8101-1	ASSY CONTROLLER TO ATTEN	1	W7		
16	074-912	KIT, RACK MOUNTING W/O HANDLES 3.5 H	1	NA	24803	K2RMX-001A
17	074-761-1	HOLE PLUG 3/8 HOLE NYLON BLACK	8	NA	83330	3091
18	074-921	FEET NON-SKID	4	NA	4963	SJ-5008 BLACK
					4963	SJ-5008SP
					24803	KFT12-BLK
19	NAS1635-04LR4	SCR PAN HD SELFLOCK 4-40 X 1/4	12	NA		
20	MS24693-C3	SCR FLAT HD 4-40 X 5/16 LG 100	8	NA		
21	090-354	* LABEL WARNING HIGH VOLTAGE	1	NA		
22	090-445	* LABEL, REFERENCE INSTR MANUAL	1	NA		
25	090-301	* LABEL STD 1.5 X .75 IN	1	NA		
26	IM501	O & S, ATTEN UNIT MODEL 8311 (+15V) W/ETHERNET	1	NA		
27	193-8148	WIRING DIAGRAM MODEL 8311-202-X-XN	0	NA		
28	089-4090	ICD, ATTEN UNIT, MODEL 8311 W/ETHERNET 150 ATTENS	0	NA		

Refer to Aeroflex / Weinschel Drawing 193-7307-6, Rev. A for parts location.

Model 8310-202-3-FN, Attenuator Unit Assembly Replaceable Parts List (P/N 193-7305-7, Rev. A):

Find No.	Part Number	Description	Quantity Used	Reference Designator	CAGE Code	Vendor Part Number
1	193-8138-1	ASSY, ATTEN, BASE UNIT, MODEL 8311 W/ETHERNET (+15V)	1	NA		
2	193-8054	OVERLAY, FRONT PANEL SMA	1	NA		
3	193-8049	OVERLAY, PANEL BLANK	1	NA		
4	193-8042	MOUNTING PLATE	2	NA		
5	193-8118	MOUNTING PLATE	1	NA		
6	150T-11	ATTEN PRGM SMARTSTEP	3	AT2, AT4, AT6		
7	150T-110	ATTEN PRGM SMARTSTEP	3	AT1, AT3, AT5		
10	1568	ADAPT WPM 3 BULKHD	6	NA		
11	068-32-4/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	3	W9, W12, W15		B068-32-4/0
12	068-32-6/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	2	W8,W10		B068-32-6/0
13	068-32-12/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	4	W11, W13, W14, W16	93459	B068-32-12/0
14	193-9646	CONNECTOR ADAPTER PLATE	6	NA		
15	193-8101-1	ASSY CONTROLLER TO ATTEN	1	W7		
16	074-912	KIT, RACK MOUNTING W/O HANDLES 3.5 H	1	NA	24803	K2RMX-001A
17	074-761-1	HOLE PLUG 3/8 HOLE NYLON BLACK	6	NA	83330	3091
18	074-921	FEET NON-SKID	4	NA	4963 4963 24803	SJ-5008 BLACK SJ-5008SP KFT12-BLK
19	NAS1635-04LR4	SCR PAN HD SELFLOCK 4-40 X 1/4	17	NA		
20	MS24693-C3	SCR FLAT HD 4-40 X 5/16 LG 100	12	NA		
21	090-354	* LABEL WARNING HIGH VOLTAGE	1	NA		
22	090-445	* LABEL, REFERENCE INSTR MANUAL	1	NA		
25	090-301	* LABEL STD 1.5 X .75 IN	1	NA		
26	IM501	O & S, ATTEN UNIT MODEL 8311 (+15V) W/ETHERNET	1	NA		
27	193-8148	WIRING DIAGRAM MODEL 8311-202-X-XN	0	NA		
28	089-4090	ICD, ATTEN UNIT, MODEL 8311 W/ETHERNET 150 ATTENS	0	NA		

Refer to Aeroflex / Weinschel Drawing 193-7307-5, Rev. A for parts location.

Model 8310-353-6-FN, Attenuator Unit Assembly Replaceable Parts List (P/N 193-7307-2, Rev. A):

Find No.	Part Number	Description	Quantity Used	Reference Designator	CAGE Code	Vendor Part Number
1	193-8138-1	ASSY, ATTEN, BASE UNIT, MODEL 8311 W/ETHERNET (+15V)	1	NA		
2	193-10265	MOUNTING PLATE	2	NA		
4	193-8054	OVERLAY, FRONT PANEL, SMA	1	NA		
5	193-8049	OVERLAY, PANEL BLANK	1	NA		
7	193-10066	SPACER, CONNECTOR, 12 POS	1	NA		
11	193-8144	ASSY, CABLE, CONTROLLER TO ATTEN	1	W11		
17	074-912	KIT, RACK MOUNTING W/O HANDLES 3.5 H	1	NA	24803	K2RMX-001A
18	090-301	* LABEL STD, 1.5 X .75 IN	1	NA		
20	3408T-103	ATTEN PRGM, SMARTSTEP	6	AT1 -AT6		
21	1568	ADAPT WPM 3 BULKHD	12	NA		
23	068-32-4/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	6	W13, W15, W17, W19, W21, W23		B068-32-4/0
24	068-32-12/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	6	W14, W16, W18, W20, W22, W24	93459	B068-32-12/0
27	NAS1635-04LR4	SCR PAN HD SELFLOCK, 4-40 X 1/4	8	NA		
28	NAS662C2LPR3	SCR, FLT HD, #2-56 X 3/16 LG, SELF-LOCK	12	NA		
29	NAS1635-04LR5	SCR PAN HD SELF LOCK 4-40X5/16	4	NA		
30	MS15795-803	WASHER FLAT .125 ID, .250 OD	4	NA		
31	090-445	* LABEL, REFERENCE, INSTR MANUAL	1	NA		
32	090-354	* LABEL WARNING HIGH VOLTAGE	1	NA		
33	193-8141	WIRING DIAGRAM ATTEN UNIT, 8311 W/ETHERNET (+15V)	0	NA		
34	089-4073	ICD, ATTEN UNIT MODEL 8311 SERIES 6 CHANNEL,W/ETHERNET	0	NA		
35	IM501	O & S MANUAL, ATTEN UNIT	1	NA		

Refer to Aeroflex / Weinschel Drawing 193-7307-2, Rev. A for parts location.

Model 8310-353-9-TN, Attenuator Unit Assembly Replaceable Parts List (P/N 193-7307-9, Rev.B):

Find No.	Part Number	Description	Quantity Used	Reference Designator	CAGE Code	Vendor Part Number
1	193-8138-1	ASSY, ATTEN, BASE UNIT, MODEL 8311 W/ETHERNET (+15V)	1	NA		
2	193-10265	MOUNTING PLATE	2	NA		
3	193-10265-1	MOUNTING PLATE	1	NA		
4	193-8046	OVERLAY, FRONT PANEL, SMA	1	NA		
5	193-8046-1	OVERLAY, REAR PANEL, SMA	1	NA		
7	193-10066	SPACER, CONNECTOR, 12 POS	2	NA		
10	193-8153	ASSY, CABLE, ATTEN TO CONTR	1	W10		
16	074-761-1	HOLE PLUG 3/8 HOLE NYLON BLACK	6	NA	83330	3091
17	074-912	KIT, RACK MOUNTING W/O HANDLES 3.5 H	1	NA	24803	K2RMX-001A
18	090-301	* LABEL STD, 1.5 X .75 IN	1	NA		
20	3408T-103	ATTEN PRGM, SMARTSTEP	9	AT1 - AT9		
21	1568	ADAPT WPM 3 BULKHD	18	NA		
23	068-32-4/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	8	W13 - W16, W21 - W24		B068-32-4/0
24	068-32-5/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	2	W25, W30	93459	B068-32-5/0
25	068-32-6/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	4	W17, W18, W26, W27		B068-32-6/0
26	068-32-7/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	4	W19 ,W20, W28, W29	93459	B068-32-7/0
27	NAS1635-04LR4	SCR PAN HD SELFLOCK, 4-40 X 1/4	14	NA		
28	NAS662C4LPR4	SCR FLAT HD SELFLOCK, 4-40 X 1/4 LG 100 DEG	18	NA		
33	193-8141	WIRING DIAGRAM	0	NA		
34	089-4193	ICD, ATTEN UNIT, MODEL 8311 SERIES 9 CHANNEL,W/ETHERNET	0	NA		
35	IM501	O & S, ATTEN UNIT, MODEL 8311 (+15V) W/ETHERNET	1	NA		

Refer to Aeroflex / Weinschel Drawing 193-7307-9, Rev. B for parts location.

Model 8310-353-12-TN, Attenuator Unit Assembly Replaceable Parts List (P/N 193-7307-12, Rev.A):

Find No.	Part Number	Description	Quantity Used	Reference Designator	CAGE Code	Vendor Part Number
1	193-8138-1	ASSY, ATTEN, BASE UNIT, MODEL 8311 W/ETHERNET (+15V)	1	NA		
2	193-10265	MOUNTING PLATE	2	NA		
3	193-10265-1	MOUNTING PLATE	1	NA		
4	193-8046	OVERLAY, FRONT PANEL SMA	1	NA		
5	193-8046-1	OVERLAY, REAR PANEL SMA	1	NA		
7	193-10066	SPACER, CONNECTOR, 12 POS	2	NA		
10	193-11271	ASSY, CABLE, 14 PIN ATTEN TO CONTR	1	W10		
16	074-761-1	HOLE PLUG 3/8 HOLE	6	NA	83330	3091
17	074-912	KIT, RACK MOUNTING, W/O HANDLES 3.5 H	1	NA	24803	K2RMX-001A
18	090-301	* LABEL STD, 1.5 X .75 IN	1	NA		
20	3408T-103	ATTEN PRGM, SMARTSTEP	12	AT1 - AT12		
21	1568	ADAPTER WPM3 BULKHD	24	NA		
22	068-32-8/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	4	W25, W26, W35, W36		B068-32-8/0
23	068-32-4/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	7	W13 - W19		B068-32-4/0
24	068-32-5/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	1	W20	93459	B068-32-5/0
25	068-32-6/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	6	W21 - W24, W31, W32		B068-32-6/0
26	068-32-7/0	COAXIAL CABLE ASSY, SMA M/M, CONFORMABLE, DC TO 18 GHz	6	W27 - W30, W33, W34	93459	B068-32-7/0
27	NAS1635-04LR4	SCR PAN HD SELFLOCK, 4-40 X 1/4	12	NA		
28	NAS662C4LPR4	SCR FLAT HD SELFLOCK, 4-40 X 1/4 LG 100 DEG	24	NA		
33	193-8141	WIRING DIAGRAM, ATTEN UNIT, 8311 W/ETHERNET (+15V)	0	NA		
34	089-4255	ICD, ATTEN UNIT, 12 CHANNEL	0	NA		
35	IM501	O & S, ATTEN UNIT, MODEL 8311 (+15V) W/ETHERNET	1	NA		

Refer to Aeroflex / Weinschel Drawing 193-7307-12, Rev. A for parts location.

Basic Model 8311-XX-X-XN (+5 V) Assembly Replaceable Parts List (P/N 193-8138, Rev. A):

Find No.	Part Number	Description	Quantity Used	Reference Designator	CAGE Code	Vendor Part Number
1	193-8142	ENCLOSURE, MODIFIED	1	NA		
2	193-8048	CHASSIS	1	NA		
5	193-10815	ASSY, CABLE, DC POWER, +5V	1	W4		
6	193-9177	ASSY CABLE PWR/INPUT TO PSU	1	W2		
7	193-8023-003	ASSY, PCB, CONTROLLER, +5V	1	A1		
10	193-8086-2	ASSY, CABLE. ATTEN TO DISTRIBUTION	1	W3		
11	193-10053-001	ASSY, PCB, 8210 XPORT ETHERNET INTF W/ D CONNECTOR	1	A5		
13	193-9236	OVERLAY	1	NA		
15	193-8029-001	ASSY, PCB, FRONT PANEL DISPLAY	1	A3		
16	193-8028-000	ASSY, PCB, CONTROL, FRONT PANEL	1	A4		
17	001-400-5	PSU SWITCHER, +5V DC, 8A	1	A2	60975	GLC50-5
18	051-40	FUSE HOLDER, POWER INPUT, W/SWITCH	1	XF1	5245	PSOSXSS6B
20	193-9193	ASSY, CABLE, CONTROLLER TO FRONT PANEL DISPLAY	1	W5		
21	193R-8137-000	ASSY, PCB, TRANSITION, 10 PIN TO 14 PIN INTERFACE	1	A6		
22	062-184-5	CONN SCREW LOCK FEMALE	2	NA	71468	M24308-26-1F
24	068-21	CORD PWR 3-CONDUCTOR DTCH 7.5FT 10A-125V NEMA5-15P/IEC320-C13	1	NA	16428	17250
30	055-117	SWITCH SLIDE SPDT ON-OFF-ON PANEL MT 6A @ 28VDC	1	S1	9353	1103M1S3ZQE2
32	090-285	*NAMEPLATE HIGH VOLTAGE	1	NA		
33	193-9159	ASSY, CABLE, GND	1	W1		
34	052-1-1/5	FUSE 1.5 AMP, 250V	1	F1	75915	312.01.5
36	MS51957-19	SCR PAN HD 4-40 X 3/4 LG	2	NA		
37	090-353	* LABEL GROUND	1	NA		
38	090-467	*LABEL, POWER INPUT	1	NA		
39	MS51957-17	SCR PAN HD 4-40 X 1/2 LG	4	NA		
40	MS15795-803	WASHER FLAT .125 ID, .250 OD	12	NA		
41	MS35338-135	WASHER LOCK #4	10	NA		
42	MS51957-14	SCR PAN HD 4-40 X 5/16 LG	4	NA		
43	MS24693-C3	SCR FLAT HD 4-40 X 5/16 LG 100	6	NA		
44	MS35649-244	NUT HEX #4	1	NA		
45	MS51957-15	SCR PAN HD 4-40 X 3/8 LG	4	NA		
46	MS51859-2	WASHER FLAT #4, NYLON	4	NA		
48	074-477-2	SPACER HH SMITH 2381	2	NA	83330	2331
50	079-147-4	WIRE #22 YELLOW, TEFLON	0.5	NA		
51	079-147-5	WIRE #22 GREEN TEFLON	0.5	NA	0	A079-147-5
52	079-147-6	WIRE #22 LIGHT BLUE TEFLON	0.5	NA		
56	NAS662C2R4	SCR FLAT HD 2-56 X 1/4 LG 100	2	NA		
57	NAS1635-04LR4	SCR PAN HD SELFLOCK 4-40 X 1/4	2	NA		
58	MS24693-C1	SCR FLAT HD 4-40 X 3/16 LG 100	2	NA		
59	NAS671C2	NUT HEX #2 CRES SMALL PATTERN	2	NA		
60	MS15795-802	WASHER FLAT .094 ID, .250 OD	2	NA		
61	NAS1676C2	WASHER LOCK #2	2	NA		
62	193-8139	WIRING DIAGRAM, ATTENN BASE UNIT, 8311 W/ENET (+5V)	0	NA		

Refer to Aeroflex / Weinschel Drawing 193-8138, Rev. A for parts location.

Basic Model 8311-XX-X-XN (+15 V) Assembly Replaceable Parts List (P/N 193-8138-1, Rev. A):

Find No.	Part Number	Description	Quantity Used	Reference Designator	CAGE Code	Vendor Part Number
1	193-8142	ENCLOSURE, MODIFIED	1	NA		
2	193-8048	CHASSIS	1	NA		
5	193-8143	ASSY, CABLE POWER + 15V	1	W4		
6	193-9177	ASSY CABLE PWR/INPUT TO PSU	1	W2		
7	193-8023-000	ASSY,PCB, CONTROLLER	1	A1		
10	193-8086-2	ASSY, CABLE. ATTEN TO DISTRIBUTION	1	W3		
11	193-10053-001	ASSY, PCB, 8210 XPORT ETHERNET INTF W/ D CONNECTOR	1	A5		
13	193-9236	OVERLAY	1	NA		
15	193-8029-001	ASSY, PCB, FRONT PANEL DISPLAY	1	A3		
16	193-8028-000	ASSY, PCB, CONTROL, FRONT PANEL	1	A4		
17	001-400-15	PSU SWITCHER, +15V DC, 3.3A	1	A2	60975	GLC50-15
18	051-40	FUSE HOLDER, POWER IN, W/SWITCH	1	XF1	5245	PSOSXSS6B
20	193-9193	ASSY, CABLE, CONTROLLER TO FRONT PANEL DISPLAY	1	W5		
22	062-184-5	CONN SCREW LOCK FEMALE	2	NA	71468	D20418-2
24	068-21	CORD PWR 3-CONDUCTOR DTCH 7.5FT 10A-125V NEMA5-15P/IEC320-C13	1	NA	16428	17250
30	055-117	SWITCH SLIDE SPDT ON-OFF-ON PANEL MT 6A @ 28VDC	1	S1	9353	1103M1S3ZQE2
32	090-285	* NAMEPLATE HIGH VOLTAGE	1	NA		
33	193-9159	ASSY, CABLE, GND	1	W1		
34	052-1-1/5	FUSE 1.5 AMP, 250V	1	F1	75915	312.01.5
36	MS51957-19	SCR PAN HD 4-40 X 3/4 LG	2	NA		
37	090-353	* LABEL GROUND	1	NA		
38	090-467	* LABEL, POWER INPUT	1	NA		
39	MS51957-17	SCR PAN HD 4-40 X 1/2 LG	4	NA		
40	MS15795-803	WASHER FLAT .125 ID, .250 OD	12	NA		
41	MS35338-135	WASHER LOCK #4	10	NA		
42	MS51957-14	SCR PAN HD 4-40 X 5/16 LG	4	NA		
43	MS24693-C3	SCR FLAT HD 4-40 X 5/16 LG 100	6	NA		
44	MS35649-244	NUT HEX #4	1	NA		
45	MS51957-15	SCR PAN HD 4-40 X 3/8 LG	4	NA		
46	MS51859-2	WASHER FLAT #4 NYLON	4	NA		
48	074-477-2	SPACER HH SMITH 2381	2	NA	83330	2331
50	079-147-4	WIRE #22 YELLOW TEFLON	0.5	NA		
51	079-147-5	WIRE #22 GREEN TEFLON	0.5	NA	0	A079-147-5
52	079-147-6	WIRE #22 LIGHT BLUE TEFLON	0.5	NA		
56	NAS662C2R4	SCR FLAT HD 2-56 X 1/4 LG 100	2	NA		
57	NAS1635-04LR4	SCR PAN HD SELFLOCK 4-40 X 1/4	2	NA		
58	MS24693-C1	SCR FLAT HD 4-40 X 3/16 LG 100	2	NA		
59	NAS671C2	NUT HEX #2 CRES SMALL PATTERN	2	NA		
60	MS15795-802	WASHER FLAT .094 ID, .250 OD	2	NA		
61	NAS1676C2	WASHER LOCK #2	2	NA		
62	193-8140	WIRING DIAGRAM, ATTEN, BASE UNIT	0	NA		

Refer to Aeroflex / Weinschel Drawing 193-8138-1, Rev. A for parts location.

8. ACCESSORIES:

Part Number	Description
193-8033-1	Rack Mounting Kit, Single Model 8310/8311
7005-X	PLANAR CROWNS® ...refer to data sheet in Appendix C for model numbers and applicable crown specifications.

9. CONTACTING AEROFLEX / WEINSCHEL:

In the event of a malfunction, contact Aeroflex / Weinschel. An apparent malfunction of an instrument or component may be diagnosed over the phone by first contacting the Customer Service Department at Aeroflex / Weinschel. DO NOT send the instrument or component back to the factory without prior authorization. When it is necessary to return an item, state the symptoms, catalog and type number of the instrument or component, and date of original purchase. Also write the Company name and your name and phone number on a card and tape the card to the item returned. Page provides further information regarding preparation of a unit for reshipment. Contact Aeroflex / Weinschel Customer Service Department as follows:

Via mail: Aeroflex / Weinschel, Inc.
5305 Spectrum Drive
Frederick, MD 21703-7362
U.S.A.

Via Telefax: 301-846-9116

Via Phone: Call TOLL FREE 800-638-2048
Toll call # 301-846-9222

Via Website: www.aeroflex.com/weinschel

Via e-mail: weinschel-sales@aeroflex.com

10. AEROFLEX / WEINSCHEL WARRANTY:

PRODUCTS - Aeroflex / Weinschel warrants each product it manufactures to be free from defects in material and workmanship under normal use and service anywhere in the world. Aeroflex / Weinschel's only obligation under this Warranty is to repair or replace, at its plant, any product or part thereof that is returned with transportation charges prepaid to Aeroflex / Weinschel by the original purchaser within ONE YEAR from the date of shipment.

The foregoing Warranty does not apply Aeroflex / Weinschel's sole opinion to products that have been subject to improper or inadequate maintenance, unauthorized modifications, misuse, or operation outside the environmental specifications for the product.

SOFTWARE PRODUCTS - Aeroflex / Weinschel software products are supplied without representation or Warranty of any kind. Aeroflex / Weinschel, therefore, assumes no responsibility and will not accept liability (consequential or otherwise) arising from the use of program materials, disk, or tape.

The Warranty period is controlled by the Warranty document furnished with each product and begins on the date of shipment. All Warranty returns must be authorized by Aeroflex / Weinschel prior to their return.

Aeroflex / Weinschel's Quality System Certified to:

INTERTEK ISO 9001:2008 ANAB ACCREDITED

Certificate No. 94-289j

© 2008-2011 Aeroflex / Weinschel, Inc.

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 09-102 VB.	06/09	
	B	ECN 10-251 RS	AUG 10	

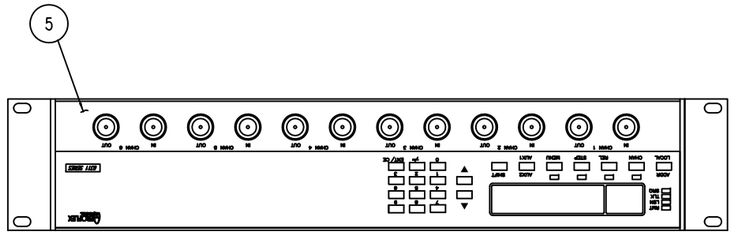

NOTES:

1. PERMANENTLY MARK NOMENCLATURE ON LABEL, ITEM 17. SEE DETAIL A.
2. APPLY LOCTITE, #242 ON ALL HARDWARE AS REQUIRED
3. AFTER ASSEMBLY CONFIGURE AND TEST

Aeroflex/Weinschel
CAGE CODE 93459 MADE IN THE USA
MODEL:8311-38-6-FN SERNO:XXX
FREQ:dc TO 2000 MHz
CHAN:6
ATTEN:63/1dB STEPS
CE

DETAIL A 1

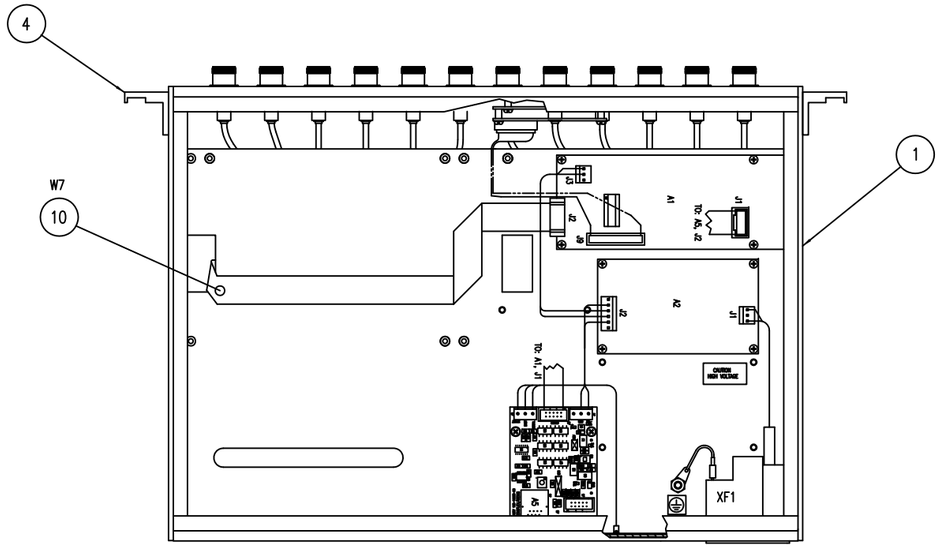

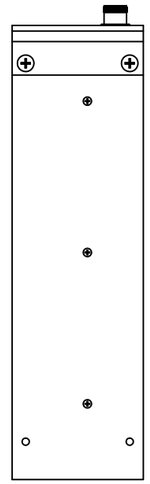

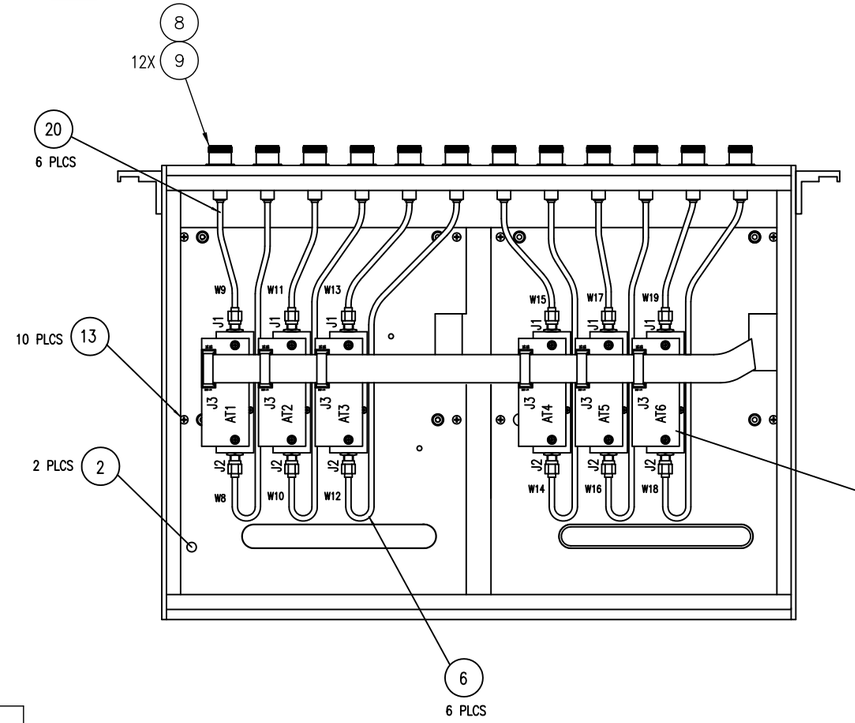

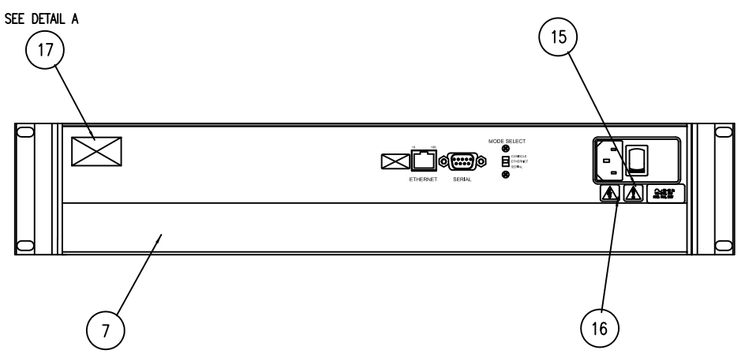

WIRING CHART			
REF DES	FROM	TO	ITEM NO.
W7	A1-J2	AT1 THRU AT6	10
W8	AT1-J2	R/P, CHAN 1 OUT	6
W9	AT1-J1	R/P, CHAN 1 IN	20
W10	AT2-J2	R/P, CHAN 2 OUT	6
W11	AT2-J1	R/P, CHAN 2 IN	20
W12	AT3-J2	R/P, CHAN 3 OUT	6
W13	AT3-J1	R/P, CHAN 3 IN	20
W14	AT4-J2	R/P, CHAN 4 OUT	6
W15	AT4-J1	R/P, CHAN 4 IN	20
W16	AT5-J2	R/P, CHAN 5 OUT	6
W17	AT5-J1	R/P, CHAN 5 IN	20
W18	AT6-J2	R/P, CHAN 6 OUT	6
W19	AT6-J1	R/P, CHAN 6 IN	20

SEE PARTS LIST PL193-7302-3

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.
PARTS LIST						

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

193-7302-3	8311-38-6-FN
NEXT ASSY	USED ON
APPLICATION	

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL N/A
FINISH N/A
DO NOT SCALE DRAWING

CONTRACT NO.

APPROVALS	DATE
DRAWN V. BETSIS	06/09
CHECKED A. HOPKINS	06/09
ENGR. W. KNILL	06/09
ISSUED	

AEROFLEX WEINSCHEL

ASSY, ATTENUATOR MODEL 8311-38-6-FN

SIZE	CAGE:	DWG. NO.	REV.
D	93459	193-7302-3	B
SCALE 1:2		SHEET 1 OF 1	

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 09-102 VB.	06/09	
	B	ECN 10-251 RS	AUG 10	

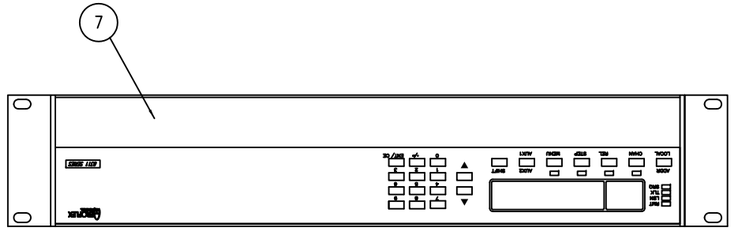

NOTES:

1. PERMANENTLY MARK NOMENCLATURE ON LABEL, ITEM 17. SEE DETAIL A.
2. APPLY LOCTITE, #242 ON ALL HARDWARE AS REQUIRED
3. AFTER ASSEMBLY CONFIGURE AND TEST

Aeroflex/Weinschel
CAGE CODE 93459 MADE IN THE USA
MODEL:8311-38-6-RN SERNO:XXX
FREQ:dc TO 2000 MHz
CHAN:6
ATTEN:63/1dB STEPS
CE

DETAIL A 1

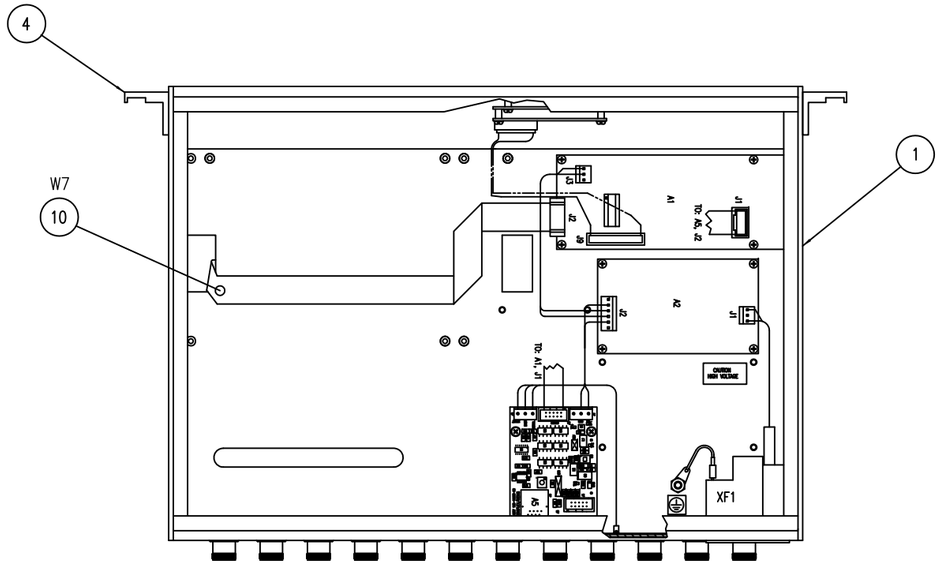

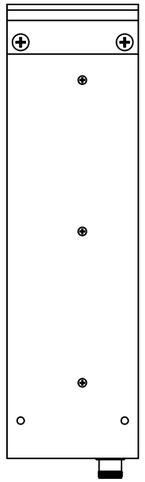

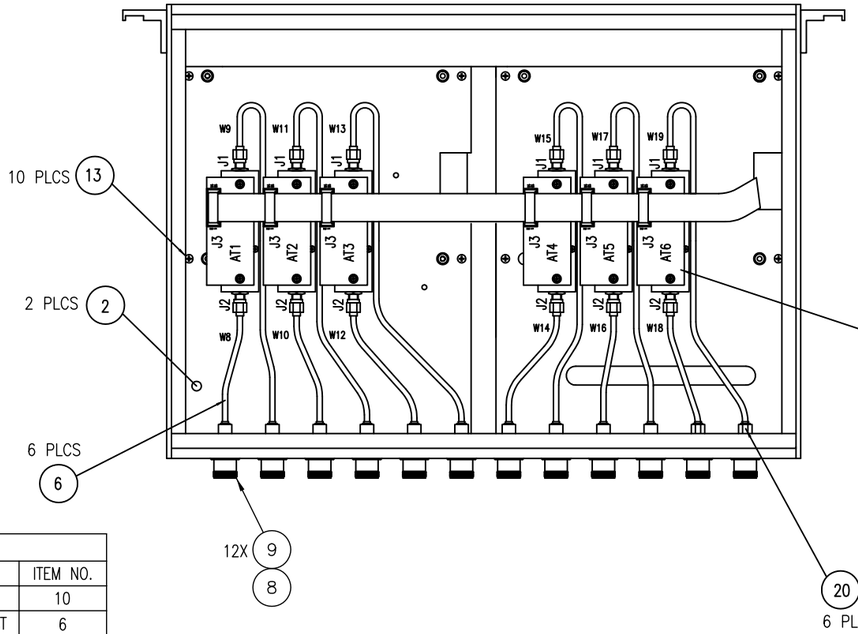

WIRING CHART			
REF DES	FROM	TO	ITEM NO.
W7	A1-J2	AT1 THRU AT6	10
W8	AT1-J2	R/P, CHAN 1 OUT	6
W9	AT1-J1	R/P, CHAN 1 IN	20
W10	AT2-J2	R/P, CHAN 2 OUT	6
W11	AT2-J1	R/P, CHAN 2 IN	20
W12	AT3-J2	R/P, CHAN 3 OUT	6
W13	AT3-J1	R/P, CHAN 3 IN	20
W14	AT4-J2	R/P, CHAN 4 OUT	6
W15	AT4-J1	R/P, CHAN 4 IN	20
W16	AT5-J2	R/P, CHAN 5 OUT	6
W17	AT5-J1	R/P, CHAN 5 IN	20
W18	AT6-J2	R/P, CHAN 6 OUT	6
W19	AT6-J1	R/P, CHAN 6 IN	20

SEE DETAIL A

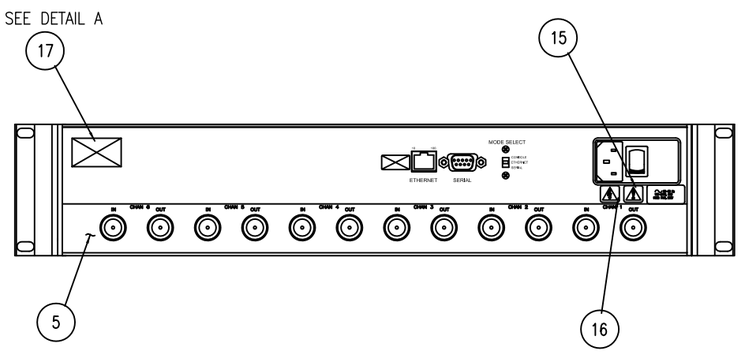

SEE PARTS LIST PL193-7302-4

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.
PARTS LIST						

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

CONTRACT NO.

AEROFLEX WEINSCHEL

APPROVALS	DATE
DRAWN V. BETSIS	06/09
CHECKED A. HOPKINS	06/09
ENGR. W. KNILL	06/09
ISSUED	

ASSY, ATTENUATOR
MODEL 8311-38-6-RN

193-7302-4	8311-38-6-RN
NEXT ASSY	USED ON
APPLICATION	

MATERIAL N/A
FINISH N/A
DO NOT SCALE DRAWING

SIZE D | CAGE: 93459 | DWG. NO. 193-7302-4 | REV. B
SCALE 1:2 | SHEET 1 OF 1

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 09-102 VB.	06/09	
	B	ECN 10-251 RS	AUG 10	

NOTES:

1. PERMANENTLY MARK NOMENCLATURE ON LABEL, ITEM 17. SEE DETAIL A.
2. APPLY LOCTITE, #242 ON ALL HARDWARE AS REQUIRED
3. AFTER ASSEMBLY CONFIGURE AND TEST

Aeroflex/Weinschel
CAGE CODE 93459 MADE IN THE USA
MODEL:8311-38-6-R-EN SERNO:XXX
FREQ:dc TO 3000 MHz
CHAN:6
ATTEN:63/1dB STEPS
CE

DETAIL A 1

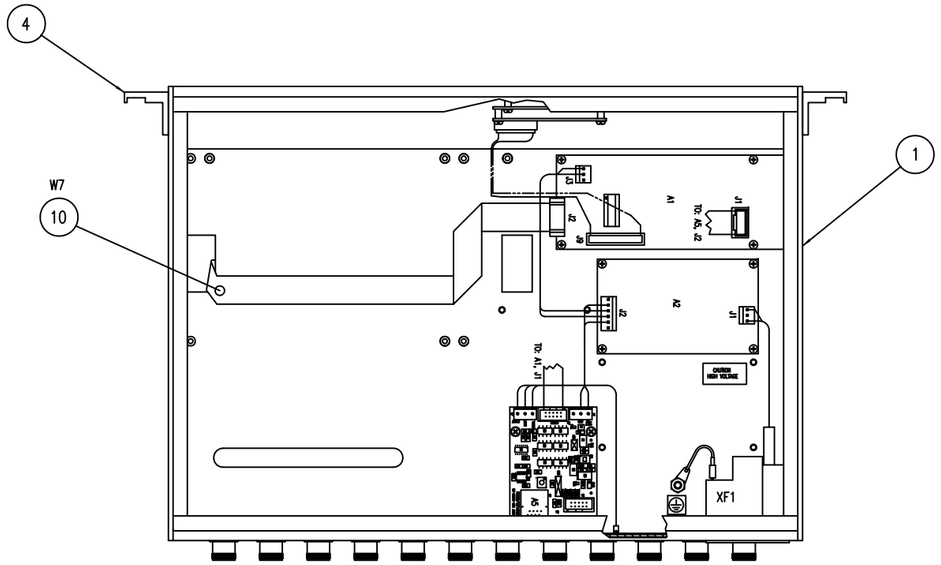

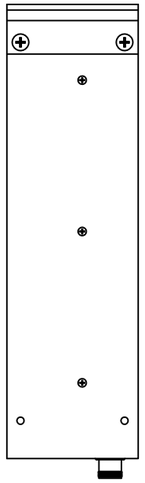

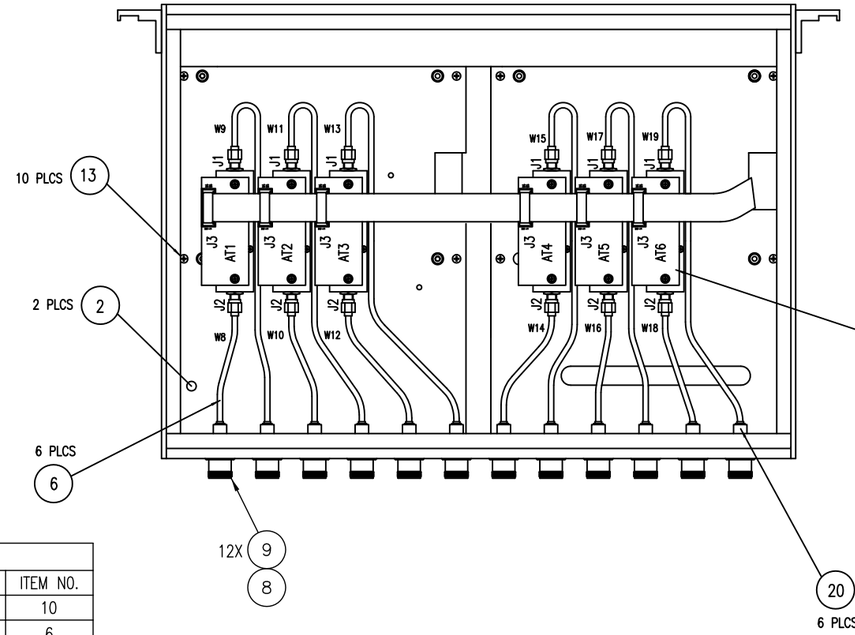

WIRING CHART			
REF DES	FROM	TO	ITEM NO.
W7	A1-J2	AT1 THRU AT6	10
W8	AT1-J2	R/P, CHAN 1 OUT	6
W9	AT1-J1	R/P, CHAN 1 IN	20
W10	AT2-J2	R/P, CHAN 2 OUT	6
W11	AT2-J1	R/P, CHAN 2 IN	20
W12	AT3-J2	R/P, CHAN 3 OUT	6
W13	AT3-J1	R/P, CHAN 3 IN	20
W14	AT4-J2	R/P, CHAN 4 OUT	6
W15	AT4-J1	R/P, CHAN 4 IN	20
W16	AT5-J2	R/P, CHAN 5 OUT	6
W17	AT5-J1	R/P, CHAN 5 IN	20
W18	AT6-J2	R/P, CHAN 6 OUT	6
W19	AT6-J1	R/P, CHAN 6 IN	20

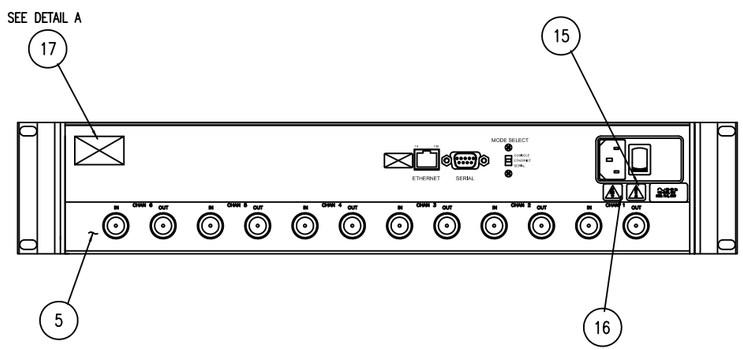

SEE PARTS LIST PL193-7302-13

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.
PARTS LIST						

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

193-7302-13	8311-38-6-R-EN
NEXT ASSY	USED ON
APPLICATION	

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL N/A
FINISH N/A
DO NOT SCALE DRAWING

CONTRACT NO.

APPROVALS	DATE
DRAWN V. BETSIS	06/09
CHECKED A. HOPKINS	06/09
ENGR. W. KNILL	06/09
ISSUED	

AEROFLEX WEINSCHEL

ASSY, ATTENUATOR
MODEL 8311-38-6-R-EN

SIZE	CAGE:	DWG. NO.	REV.
D	93459	193-7302-13	B
SCALE 1:2		SHEET 1 OF 1	

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS

ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 09-102 GT	06/09	

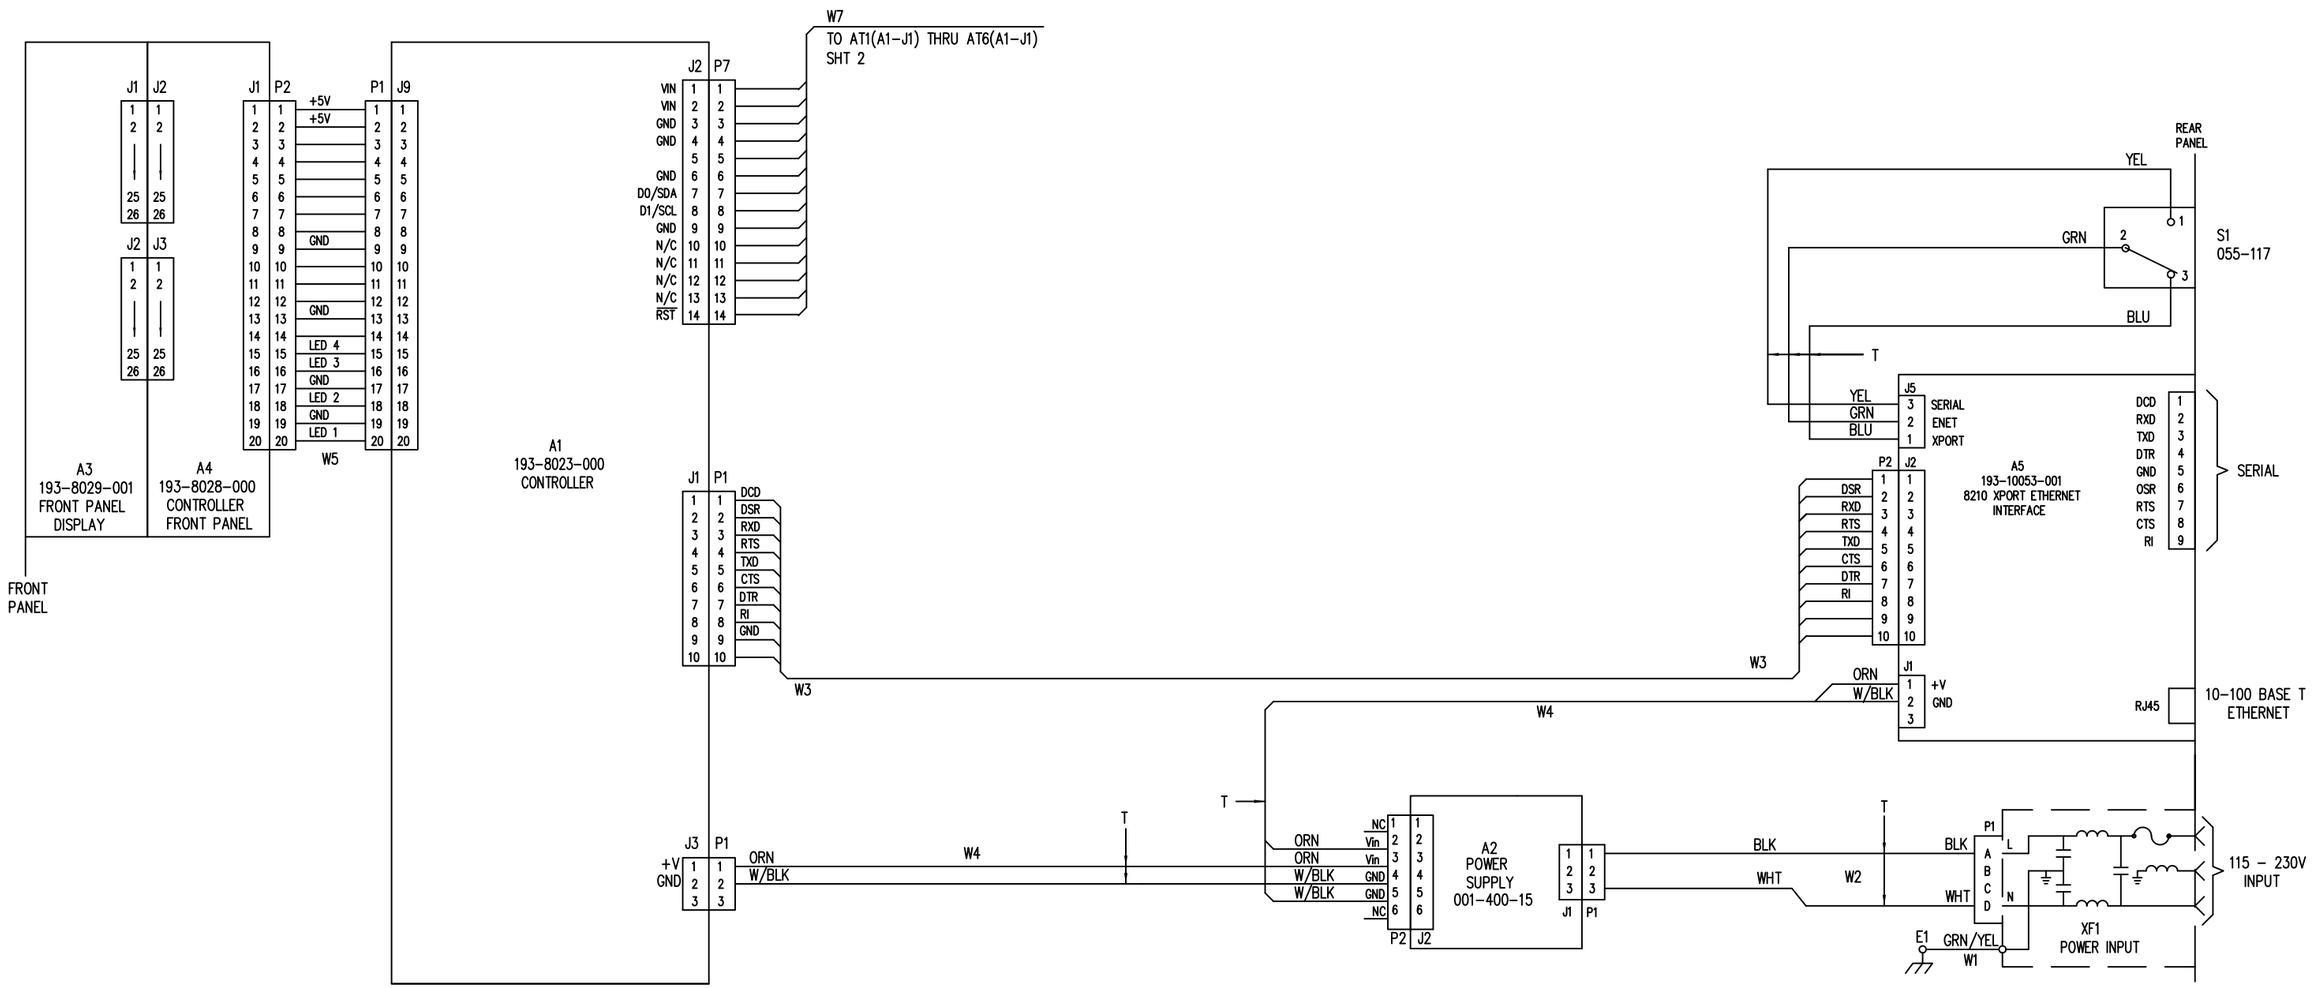

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.

PARTS LIST

193-7302-3	8311-38-6-FN
193-7302-4	8311-38-6-RN
193-7302-13	8311-38-6-R-EN
NEXT ASSY	USED ON
APPLICATION	

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL

FINISH

DO NOT SCALE DRAWING

CONTRACT NO.

APPROVALS	DATE
DRAWN G. THOMAS	06/09
CHECKED A. HOPKINS	06/09
ENGR. W. KNILL	06/09
ISSUED	

AEROFLEX WEINSCHEL

WIRING DIAGRAM, ATTEN UNIT
8311-38-X-X W/ETHERNET (+15V)

SIZE	CAGE:	DWG. NO.	REV.
D	93459	193-8150	A

SCALE NONE SHEET 1 OF 2

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 08-128 M.T.	08/08	

NOTES:

1. PERMANENTLY MARK MODEL NUMBER, SERIAL NUMBER AND NUMBER OF CHANNELS ON LABEL, ITEM 25. SEE DETAIL A.
2. AFTER ASSEMBLY, CONFIGURE AND TEST.
3. APPLY LOCTITE ON ALL HARDWARE AS REQUIRED

W16	AT6	CHAN 3 OUT	ITEM 13
W15	AT5	AT6	ITEM 11
W14	CHAN 3 IN	AT5	ITEM 13
W13	AT4	CHAN 2 OUT	ITEM 13
W12	AT3	AT4	ITEM 11
W11	CHAN 2 IN	AT3	ITEM 13
W10	AT2	CHAN 1 OUT	ITEM 12
W9	AT1	AT2	ITEM 11
W8	CHAN 1 IN	AT1	ITEM 12
W7	A1-J2	AT1 THRU AT6	ITEM 15
DES	FROM	TO	REMARKS

CABLE CHART
193-7305-5

W13	AT4	CHAN 2 OUT	ITEM 13
W12	AT3	AT4	ITEM 11
W11	CHAN 2 IN	AT3	ITEM 13
W10	AT2	CHAN 1 OUT	ITEM 12
W9	AT1	AT2	ITEM 11
W8	CHAN 1 IN	AT1	ITEM 12
W7	A1-J2	AT1 THRU AT4	ITEM 15
DES	FROM	TO	REMARKS

CABLE CHART
193-7305-4

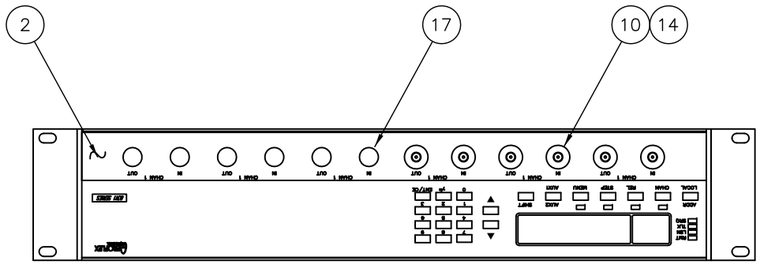

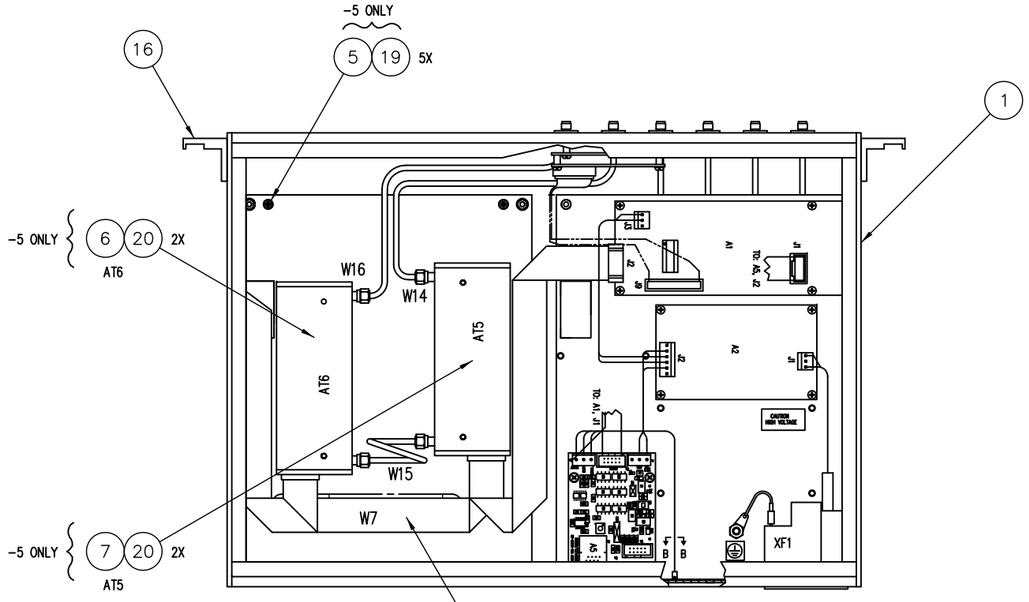

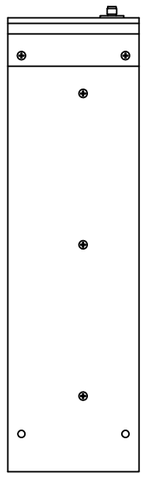

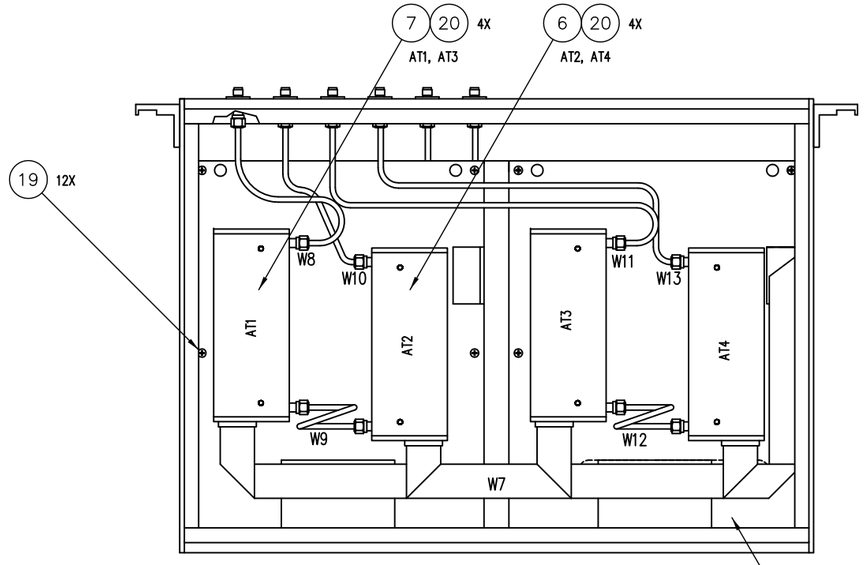

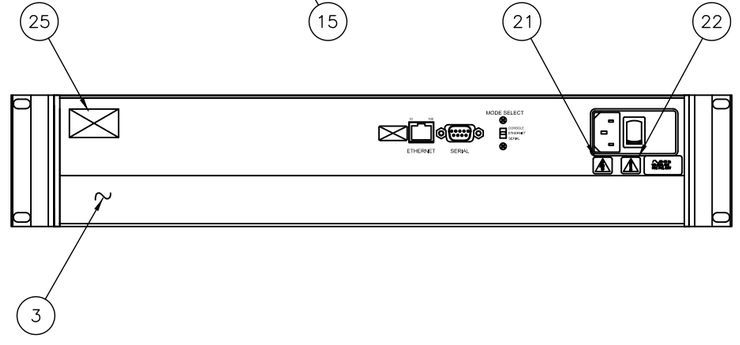

Aeroflex / Weinschel
CAGE CODE 93459 MADE IN THE USA
MODEL: SERNO:
FREQ: dc to 18GHz
CHAN: X
ATTEN: 121/1dB STEPS

DETAIL A
1

8311-202-3-FN 8311-202-2-FN	193-7305-5 193-7305-4
MODEL NUMBER	PARTS LIST

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.
PARTS LIST						

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

CONTRACT NO.

AEROFLEX WEINSCHEL

APPROVALS	DATE
DRAWN M. TYSON	08/08
CHECKED A. HOPKINS	08/08
ENGR. W. KNILL	08/08
ISSUED	

ASSY, ATTENUATOR UNIT
MODEL 8311-202-X-FN

MATERIAL N/A
FINISH N/A
DO NOT SCALE DRAWING

NEXT ASSY	USED ON
APPLICATION	

SIZE D | CAGE: 93459 | DWG. NO. 193-7305-4, -5 | REV. A
SCALE 1:2 | SHEET 1 OF 1

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 08-128 M.T.	08/08	

NOTES:

1. PERMANENTLY MARK MODEL NUMBER, SERIAL NUMBER AND NUMBER OF CHANNELS ON LABEL, ITEM 25. SEE DETAIL A.
2. AFTER ASSEMBLY, CONFIGURE AND TEST.
3. APPLY LOCTITE ON ALL HARDWARE AS REQUIRED

W16	AT6	CHAN 3 OUT	ITEM 13
W15	AT5	AT6	ITEM 11
W14	CHAN 3 IN	AT5	ITEM 13
W13	AT4	CHAN 2 OUT	ITEM 13
W12	AT3	AT4	ITEM 11
W11	CHAN 2 IN	AT3	ITEM 13
W10	AT2	CHAN 1 OUT	ITEM 12
W9	AT1	AT2	ITEM 11
W8	CHAN 1 IN	AT1	ITEM 12
W7	A1-J2	AT1 THRU AT6	ITEM 15
DES	FROM	TO	REMARKS

CABLE CHART
193-7305-7

W13	AT4	CHAN 2 OUT	ITEM 13
W12	AT3	AT4	ITEM 11
W11	CHAN 2 IN	AT3	ITEM 13
W10	AT2	CHAN 1 OUT	ITEM 12
W9	AT1	AT2	ITEM 11
W8	CHAN 1 IN	AT1	ITEM 12
W7	A1-J2	AT1 THRU AT4	ITEM 15
DES	FROM	TO	REMARKS

CABLE CHART
193-7305-6

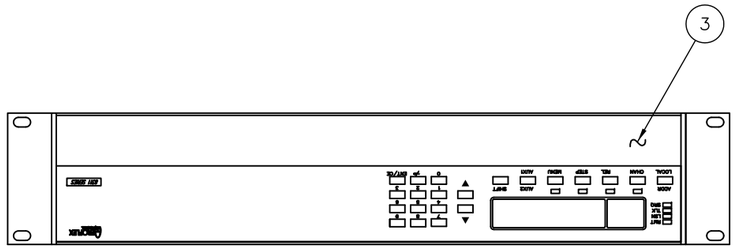

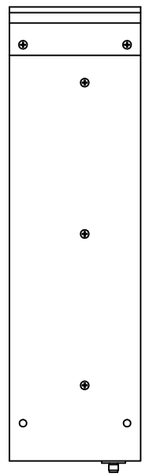

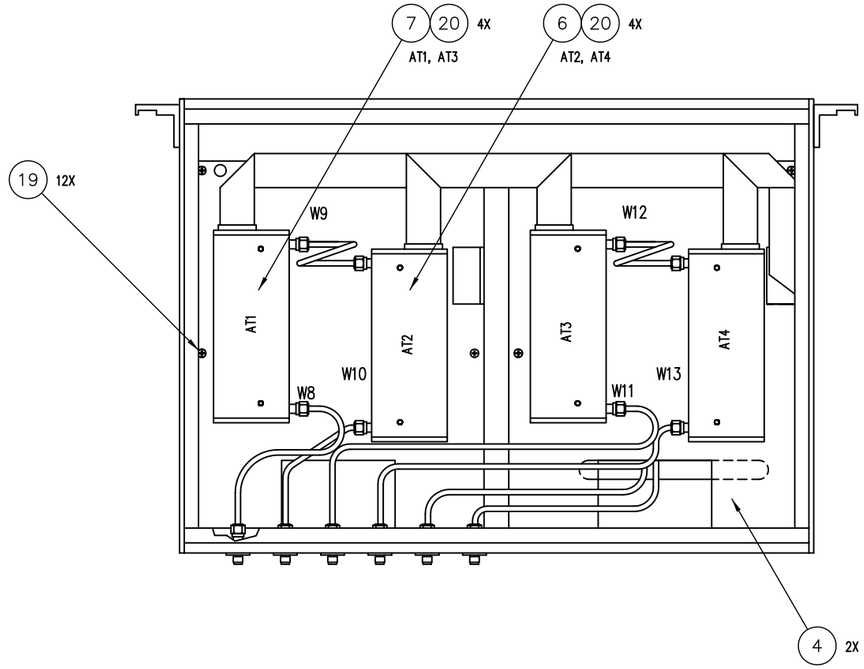

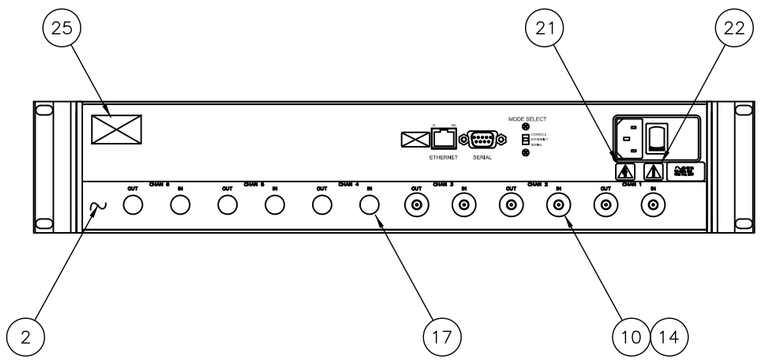

Aeroflex / Weinschel
CAGE CODE 93459 MADE IN THE USA
MODEL: SERNO:
FREQ: dc to 18GHz
CHAN: X
ATTEN: 121/1dB STEPS

DETAIL A
1

8311-202-3-RN 8311-202-2-RN	193-7305-7 193-7305-6
MODEL NUMBER	PARTS LIST

ITEM NO.	QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE

PARTS LIST

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2

CONTRACT NO.

APPROVALS	DATE
DRAWN M. TYSON	08/08
CHECKED A. HOPKINS	08/08
ENGR. W. KNILL	08/08
ISSUED	

AEROFLEX WEINSCHEL

ASSY, ATTENUATOR UNIT
MODEL 8311-202-X-RN

MATERIAL N/A
FINISH N/A
DO NOT SCALE DRAWING

NEXT ASSY	USED ON
.	.
APPLICATION	

SIZE D | CAGE: 93459 | DWG. NO. 193-7305-6, -7 | REV. A
SCALE 1:2 | SHEET 1 OF 1

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

AUTOCAD V.2007

NOTES:

1. ATTENUATORS AT1 THROUGH AT6 AND RF CABLES W8, W10, W11, W13 W14, W16 INSTALLED AS REQUIRED OUT FRONT OR REAR PANEL.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 08-128 MT.	08/08	

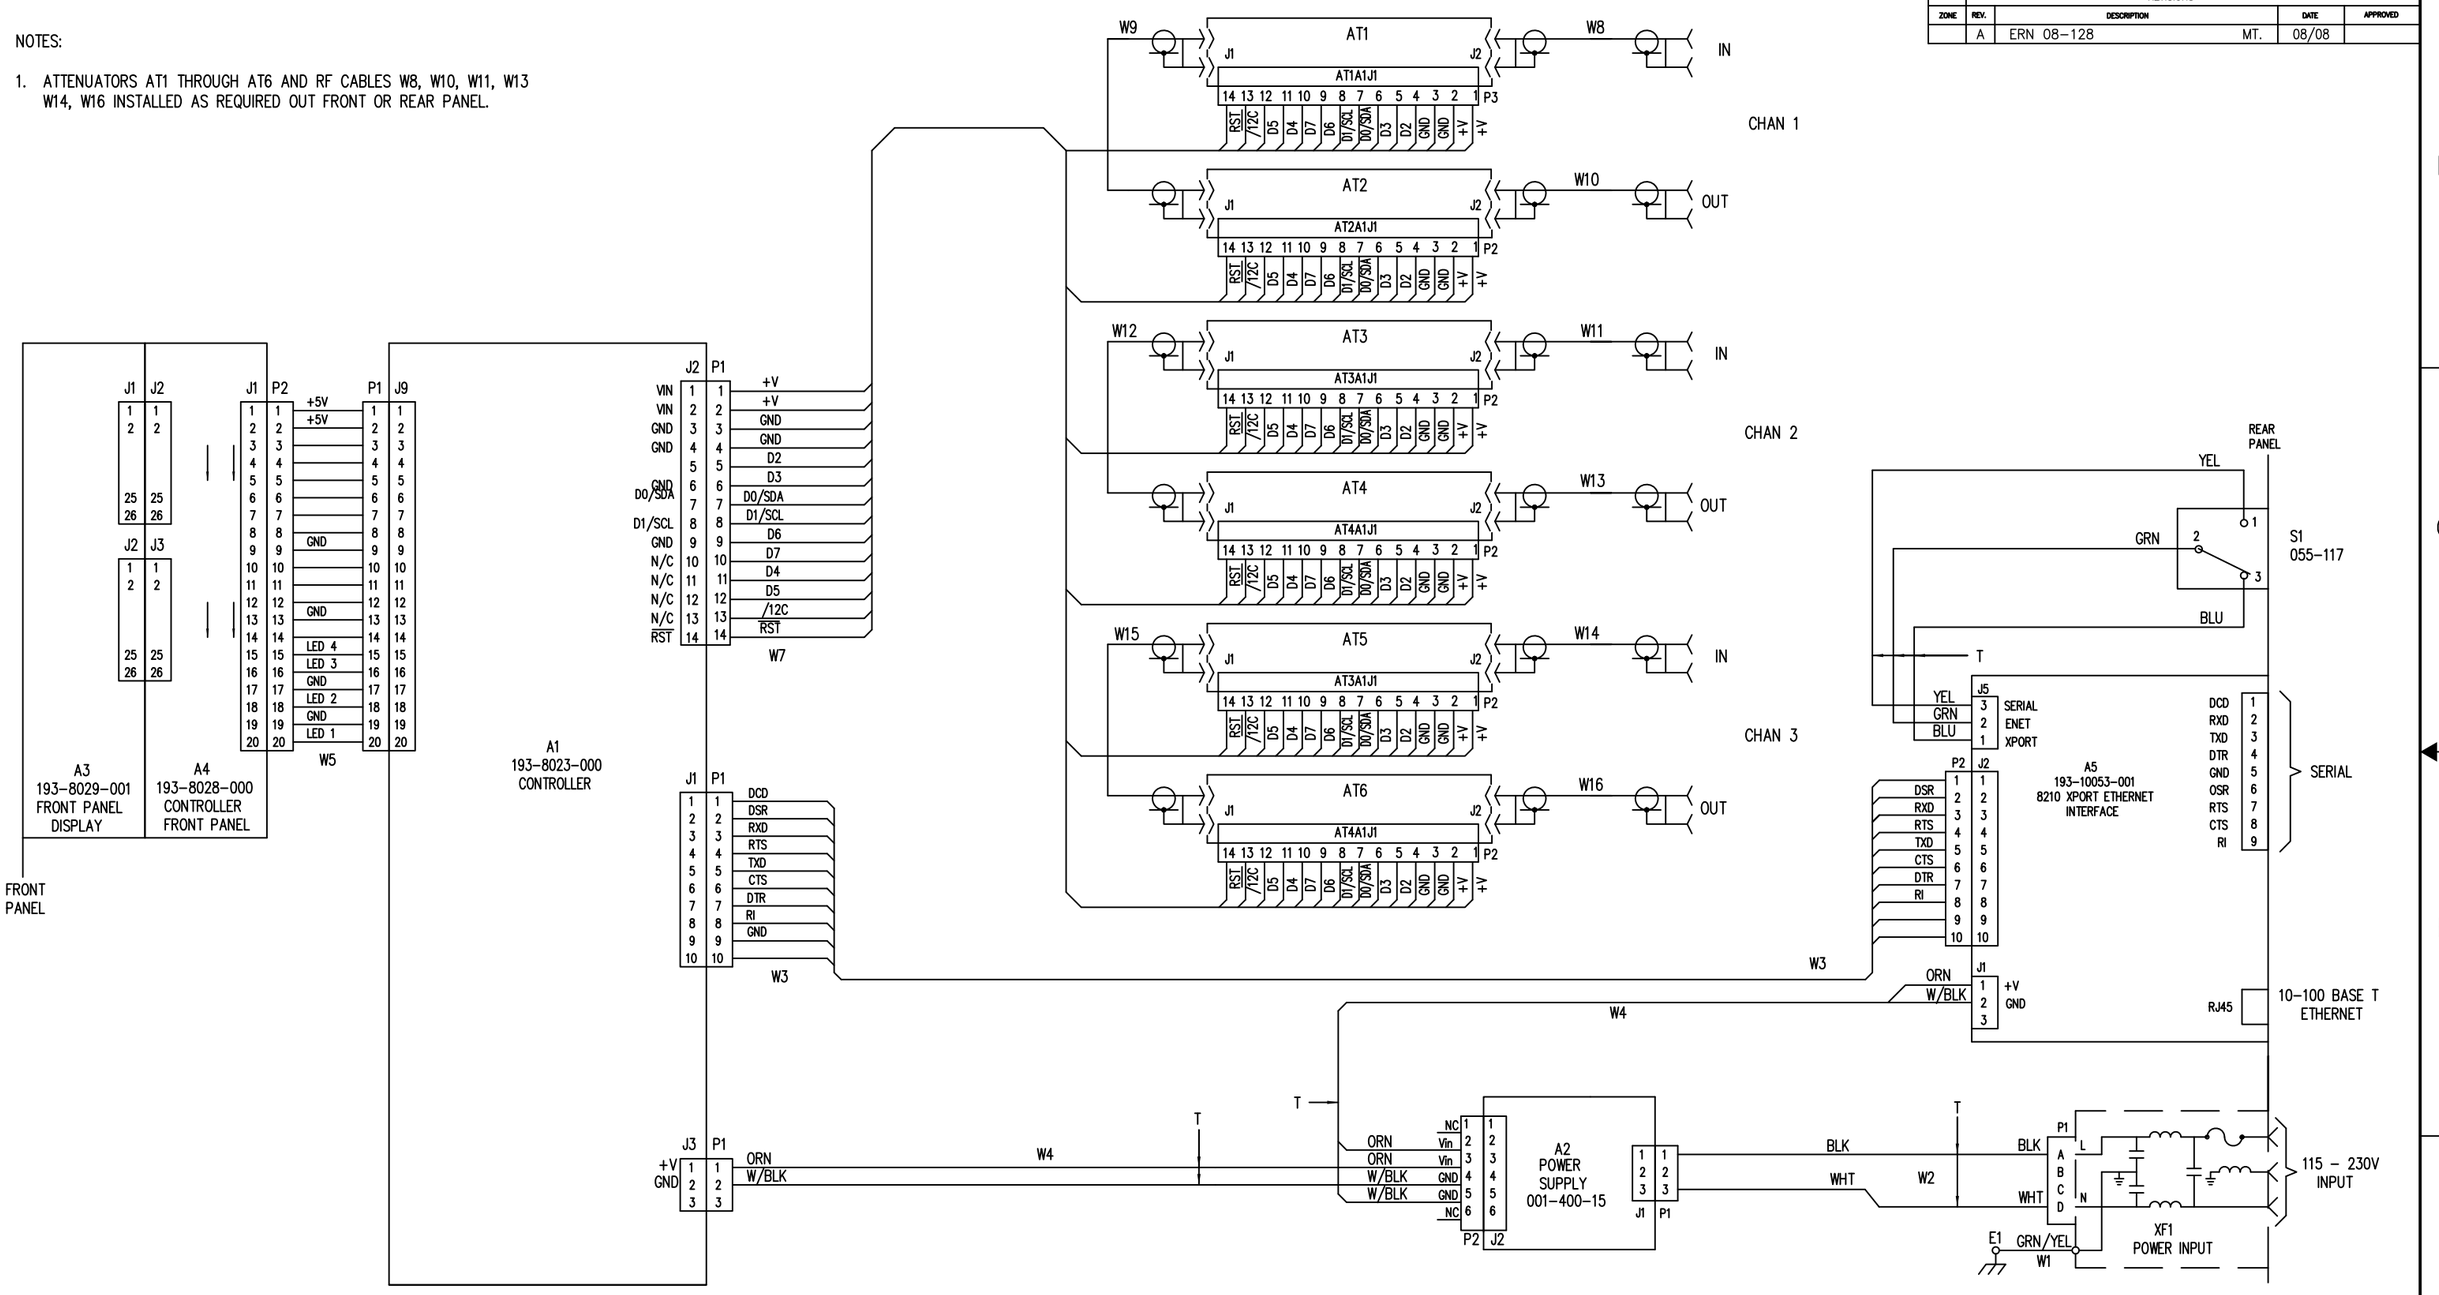

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.
PARTS LIST						
		193-7305-7				
		193-7305-6				
		193-7305-5				
	8311	193-7305-4				
NEXT ASSY	USED ON	APPLICATION				

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°
MATERIAL
FINISH
DO NOT SCALE DRAWING

CONTRACT NO.

APPROVALS	DATE
DRAWN M. TYSON	08/08
CHECKED A. HOPKINS	08/08
ENGR. W. KNILL	08/08
ISSUED	

AEROFLEX WEINSCHEL

WIRING DIAGRAM
MODEL 8311-202-X-XN

SIZE	CAGE:	DWG. NO.	REV.
D	93459	193-8148	A
SCALE NONE		SHEET 1 OF 1	

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS

ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 08-091 VB.	06/08	

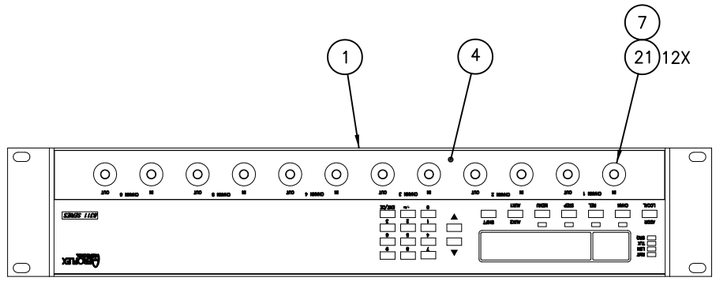

NOTES:

1. AFTER ASSEMBLY, CONFIGURE AND TEST.
2. PERMANENTLY MARK MODEL NO., SERIAL NO. & NO. OF CHANNELS ON LABEL, ITEM 18, SEE DETAIL A.

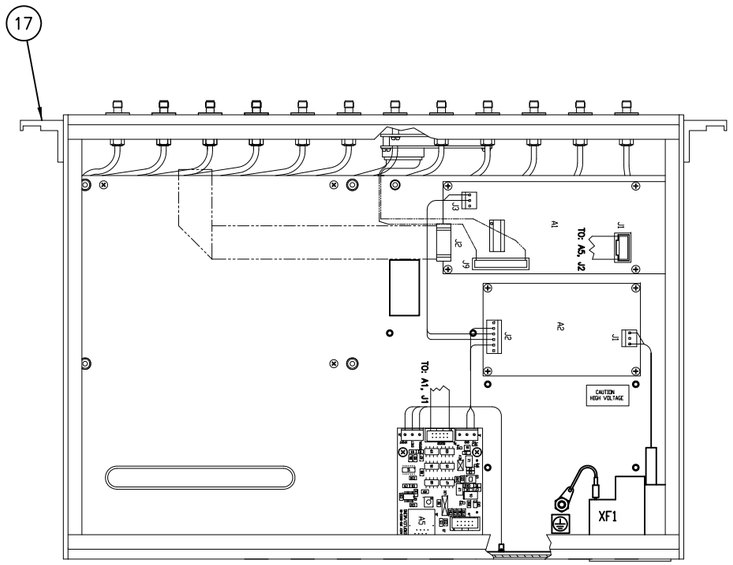

TOP VIEW

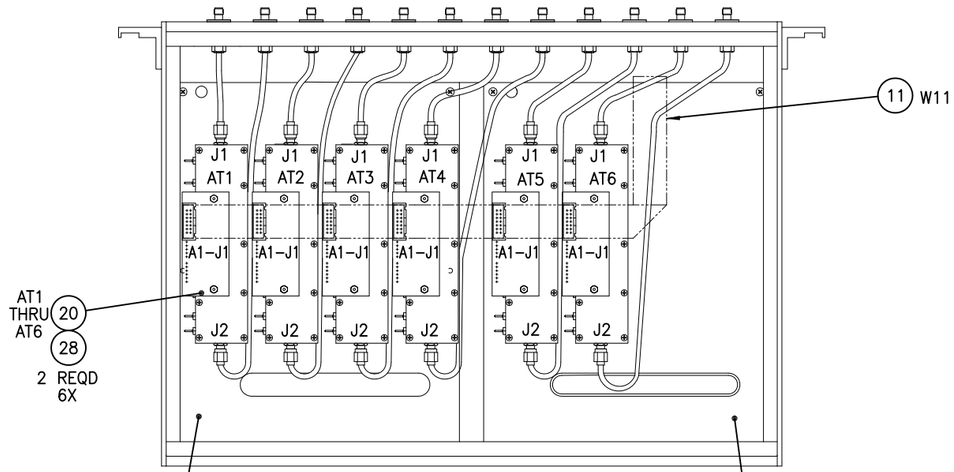

BOTTOM VIEW

W24	AT6-J2	CHAN 6 (OUT)
W23	AT6-J1	CHAN 6 (IN)
W22	AT5-J2	CHAN 5 (OUT)
W21	AT5-J1	CHAN 5 (IN)
W20	AT4-J1	CHAN 4 (OUT)
W19	AT4-J1	CHAN 4 (IN)
W18	AT3-J2	CHAN 3 (OUT)
W17	AT3-J1	CHAN 3 (IN)
W16	AT2-J2	CHAN 2 (OUT)
W15	AT2-J1	CHAN 2 (IN)
W14	AT1-J2	CHAN 1 (OUT)
W13	AT1-J1	CHAN 1 (IN)
W11	AT1(A1-J1) THRU AT6(A1-J1)	A1-J2
DES	FROM	TO

FOR PARTS LIST SEE PL193-7307-2

Aeroflex/Weinschel
CAGE CODE 93459 MADE IN THE USA
MODEL:8311-352-6-FN SERNO:
FREQ: DC TO 6.0 GHz
CHAN: 6
ATTEN: 103/1dB STEPS

VIEW A

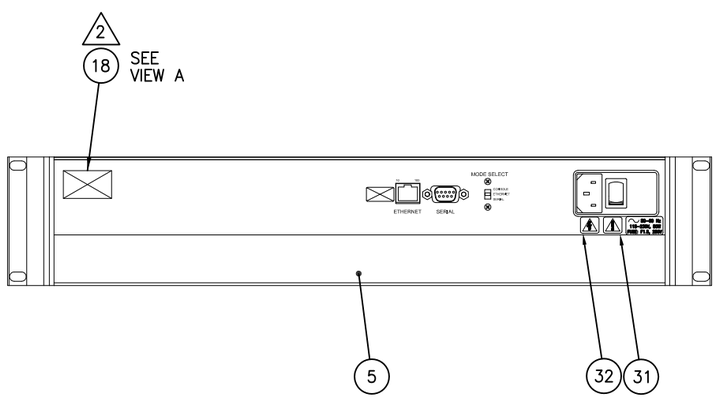

PROPRIETARY NOTICE

THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.
			PARTS LIST			

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

CONTRACT NO.

Aeroflex / Weinschel

APPROVALS		DATE
DRAWN	V. BETSIS	06/08
CHECKED	A. HOPKINS	06/08
ENGR.	W. KNILL	06/08
ISSUED		

ATTEN UNIT
6 CHANNEL W/ETHERNET

NEXT ASSY	USED ON
	8311-352-6-FN

APPLICATION

MATERIAL

FINISH

DO NOT SCALE DRAWING

SIZE	FSCM NO.	DWG. NO.	REV.
D	93459	193-7307-2	A

SCALE 1 : 2 SHEET 1 OF 1

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 09-218 R.S.	DEC 09	
	B	ECN 10-237 R.S.	AUG 10	

NOTES: UNLESS OTHERWISE SPECIFIED.

1. AFTER ASSEMBLY, CONFIGURE AND TEST.
2. PERMANENTLY MARK MODEL NO., SERIAL NO. & NO. OF CHANNELS ON LABEL, ITEM 18, SEE DETAIL A.

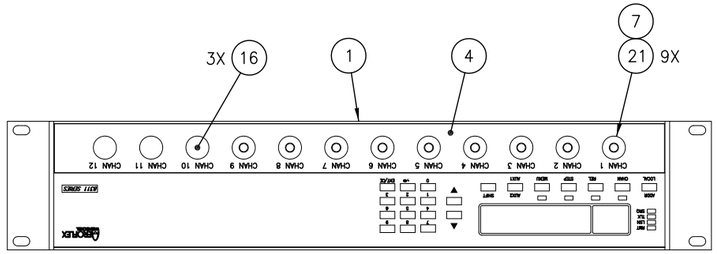

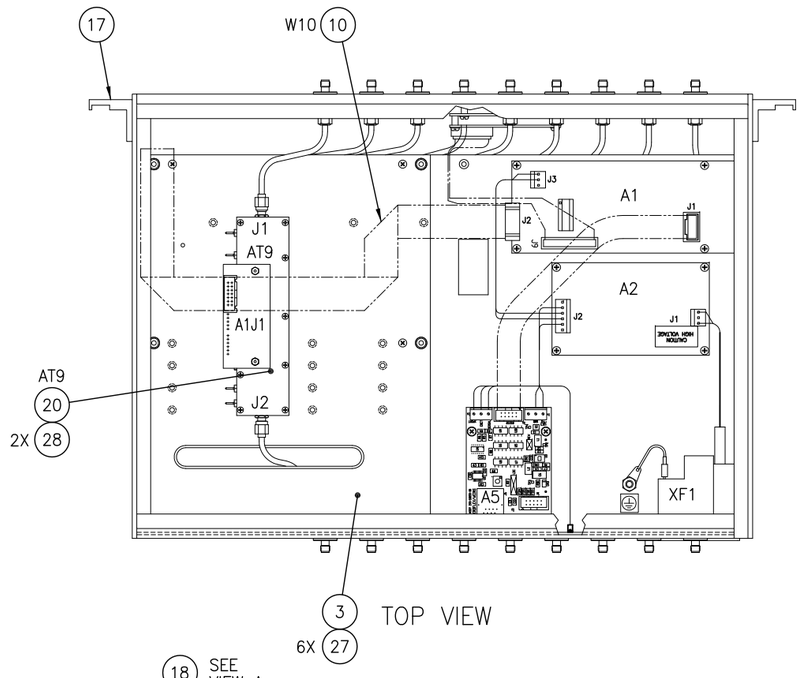

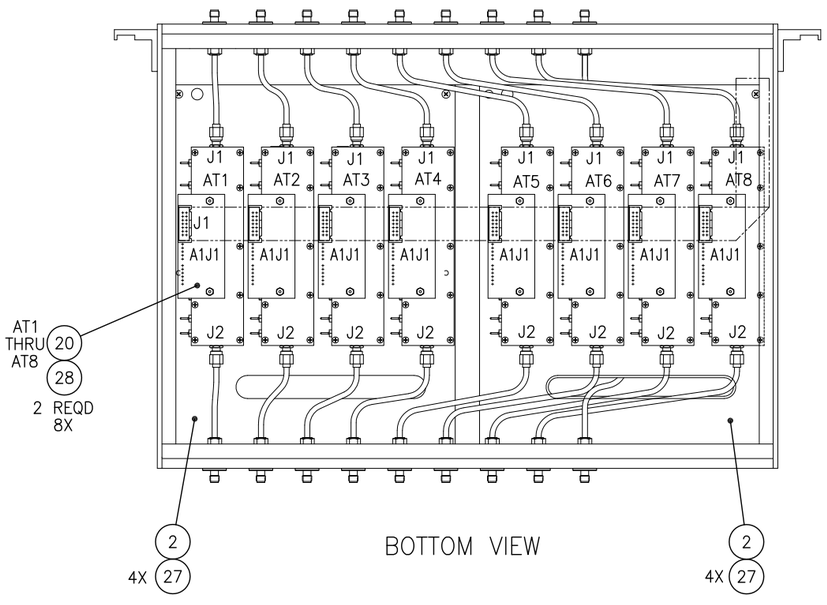

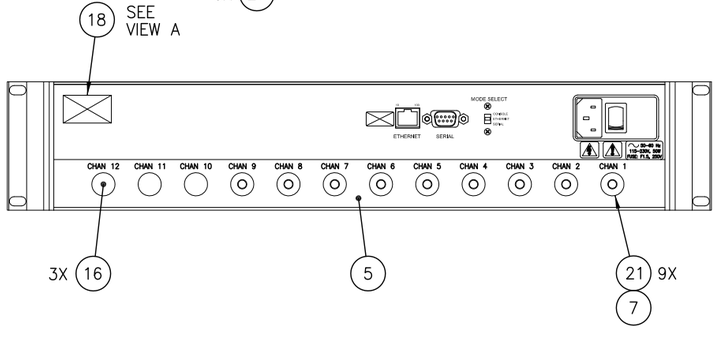

W30	AT9-J2	CHAN 9 (REAR PNL)	
W29	AT9-J1	CHAN 9 (FRONT PNL)	
W28	AT8-J2	CHAN 8 (REAR PNL)	
W27	AT8-J1	CHAN 8 (FRONT PNL)	
W26	AT7-J2	CHAN 7 (REAR PNL)	
W25	AT7-J1	CHAN 7 (FRONT PNL)	
W24	AT6-J2	CHAN 6 (REAR PNL)	
W23	AT6-J1	CHAN 6 (FRONT PNL)	
W22	AT5-J2	CHAN 5 (REAR PNL)	
W21	AT5-J1	CHAN 5 (FRONT PNL)	
W20	AT4-J2	CHAN 4 (REAR PNL)	
W19	AT4-J1	CHAN 4 (FRONT PNL)	
W18	AT3-J2	CHAN 3 (REAR PNL)	
W17	AT3-J1	CHAN 3 (FRONT PNL)	
W16	AT2-J2	CHAN 2 (REAR PNL)	
W15	AT2-J1	CHAN 2 (FNT PNL)	
W14	AT1-J2	CHAN 1 (REAR PNL)	
W13	AT1-J1	CHAN 1 (FNT PNL)	
W12	NOT USED		
W11			
W10	A1J2	AT1-A1J1 THRU AT9-A1J1	
DES	FROM	TO	

FOR PARTS LIST SEE PL193-7307-9

Aeroflex/Weinschel
CAGE CODE 93459 MADE IN THE USA
MODEL:8311-352-9-TN SERNO:
FREQ: DC TO 6.0 GHz
CHAN: 9
ATTEN: 103/1dB STEPS

VIEW A 2

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.
PARTS LIST						

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

CONTRACT NO.

Aeroflex / Weinschel

ATTEN UNIT
9 CHANNEL

APPROVALS	DATE
DRAWN R. SHOCK	1 DEC 09
CHECKED A. HOPKINS	DEC 09
ENGR. B. KNILL	DEC 09
ISSUED	

MATERIAL .
FINISH .
DO NOT SCALE DRAWING

NEXT ASSY	USED ON
.	8311-352-9-TN
APPLICATION	

SIZE D | FSCM NO. 93459 | DWG. NO. 193-7307-9 | REV. B
SCALE 1/1 | SHEET 1 OF 1

DWG. NO.	SH	REV.

REVISIONS

ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 08-169 VB.	10/08	

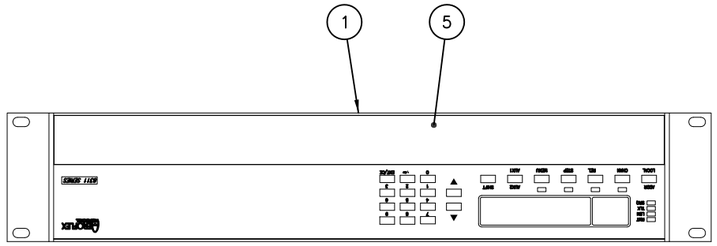

NOTES:

1. AFTER ASSEMBLY, CONFIGURE AND TEST.
2. PERMANENTLY MARK MODEL NO., SERIAL NO. & NO. OF CHANNELS ON LABEL, ITEM 18, SEE DETAIL A.

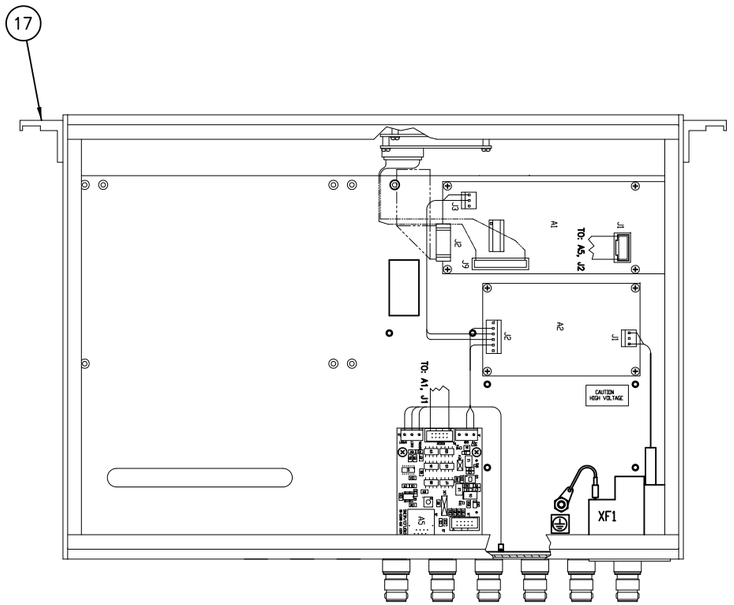

TOP VIEW

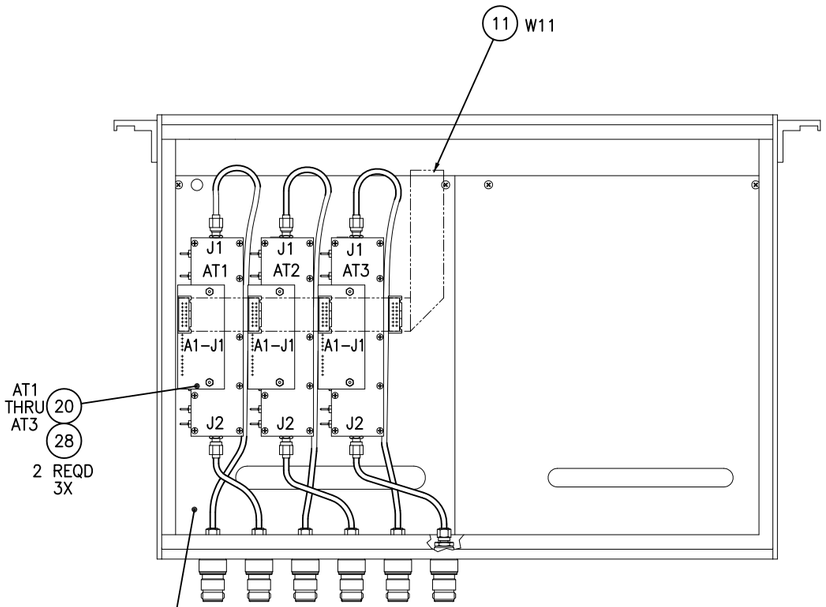

BOTTOM VIEW

Aeroflex/Weinschel
CAGE CODE 93459 MADE IN THE USA
MODEL: 8311-352-3-RNN SERNO:
FREQ: DC TO 6.0 GHz
CHAN: 3
ATTEN: 103/1dB STEPS

VIEW A

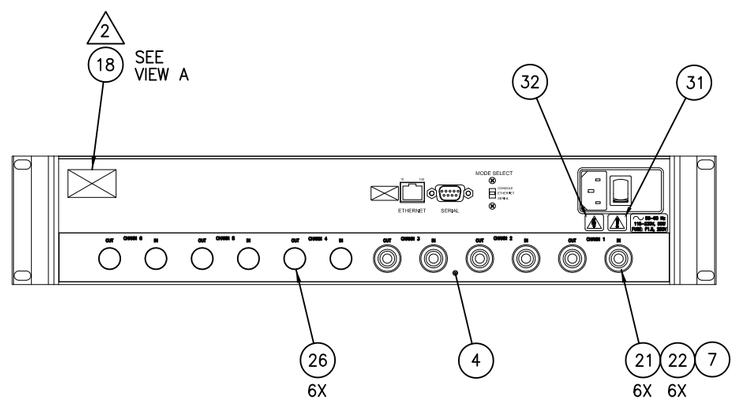

W17	AT3-J1	CHAN 3 (IN)	24
W18	AT3-J2	CHAN 3 (OUT)	25
W15	AT2-J1	CHAN 2 (IN)	24
W16	AT2-J2	CHAN 2 (OUT)	23
W13	AT1-J1	CHAN 1 (IN)	24
W14	AT1-J2	CHAN 1 (OUT)	23
W11	AT1(A1-J1) THRU AT3(A1-J1)	A1-J2	11
DES	FROM	TO	ITEM #

FOR PARTS LIST SEE PL193-7307-12

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.

PARTS LIST

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ±.01 .XXX ±.003 ANGLES ± 1/2°

CONTRACT NO.

Aeroflex / Weinschel

APPROVALS	DATE
DRAWN V. BETSIS	10/08
CHECKED A. HOPKINS	10/08
ENGR. W. KNILL	10/08
ISSUED	

ATTEN UNIT
3 CHANNEL W/ETHERNET

NEXT ASSY	USED ON
	8311-352-3-RNN

APPLICATION

MATERIAL
FINISH
DO NOT SCALE DRAWING

SIZE	FSCM NO.	DWG. NO.	REV.
D	93459	193-7307-12	A

SCALE 1 : 2 SHEET 1 OF 1

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 08–091 VB.	06/08	
	B	ECN 10–237 RS	AUG 10	

NOTES:

1. ATTENUATOR AT1–AT12 AND CABLES W13 THRU W36, INSTALLED AS REQUIRED AND CONNECT TO EITHER FRONT OR REAR PANEL AS REQUIRED.

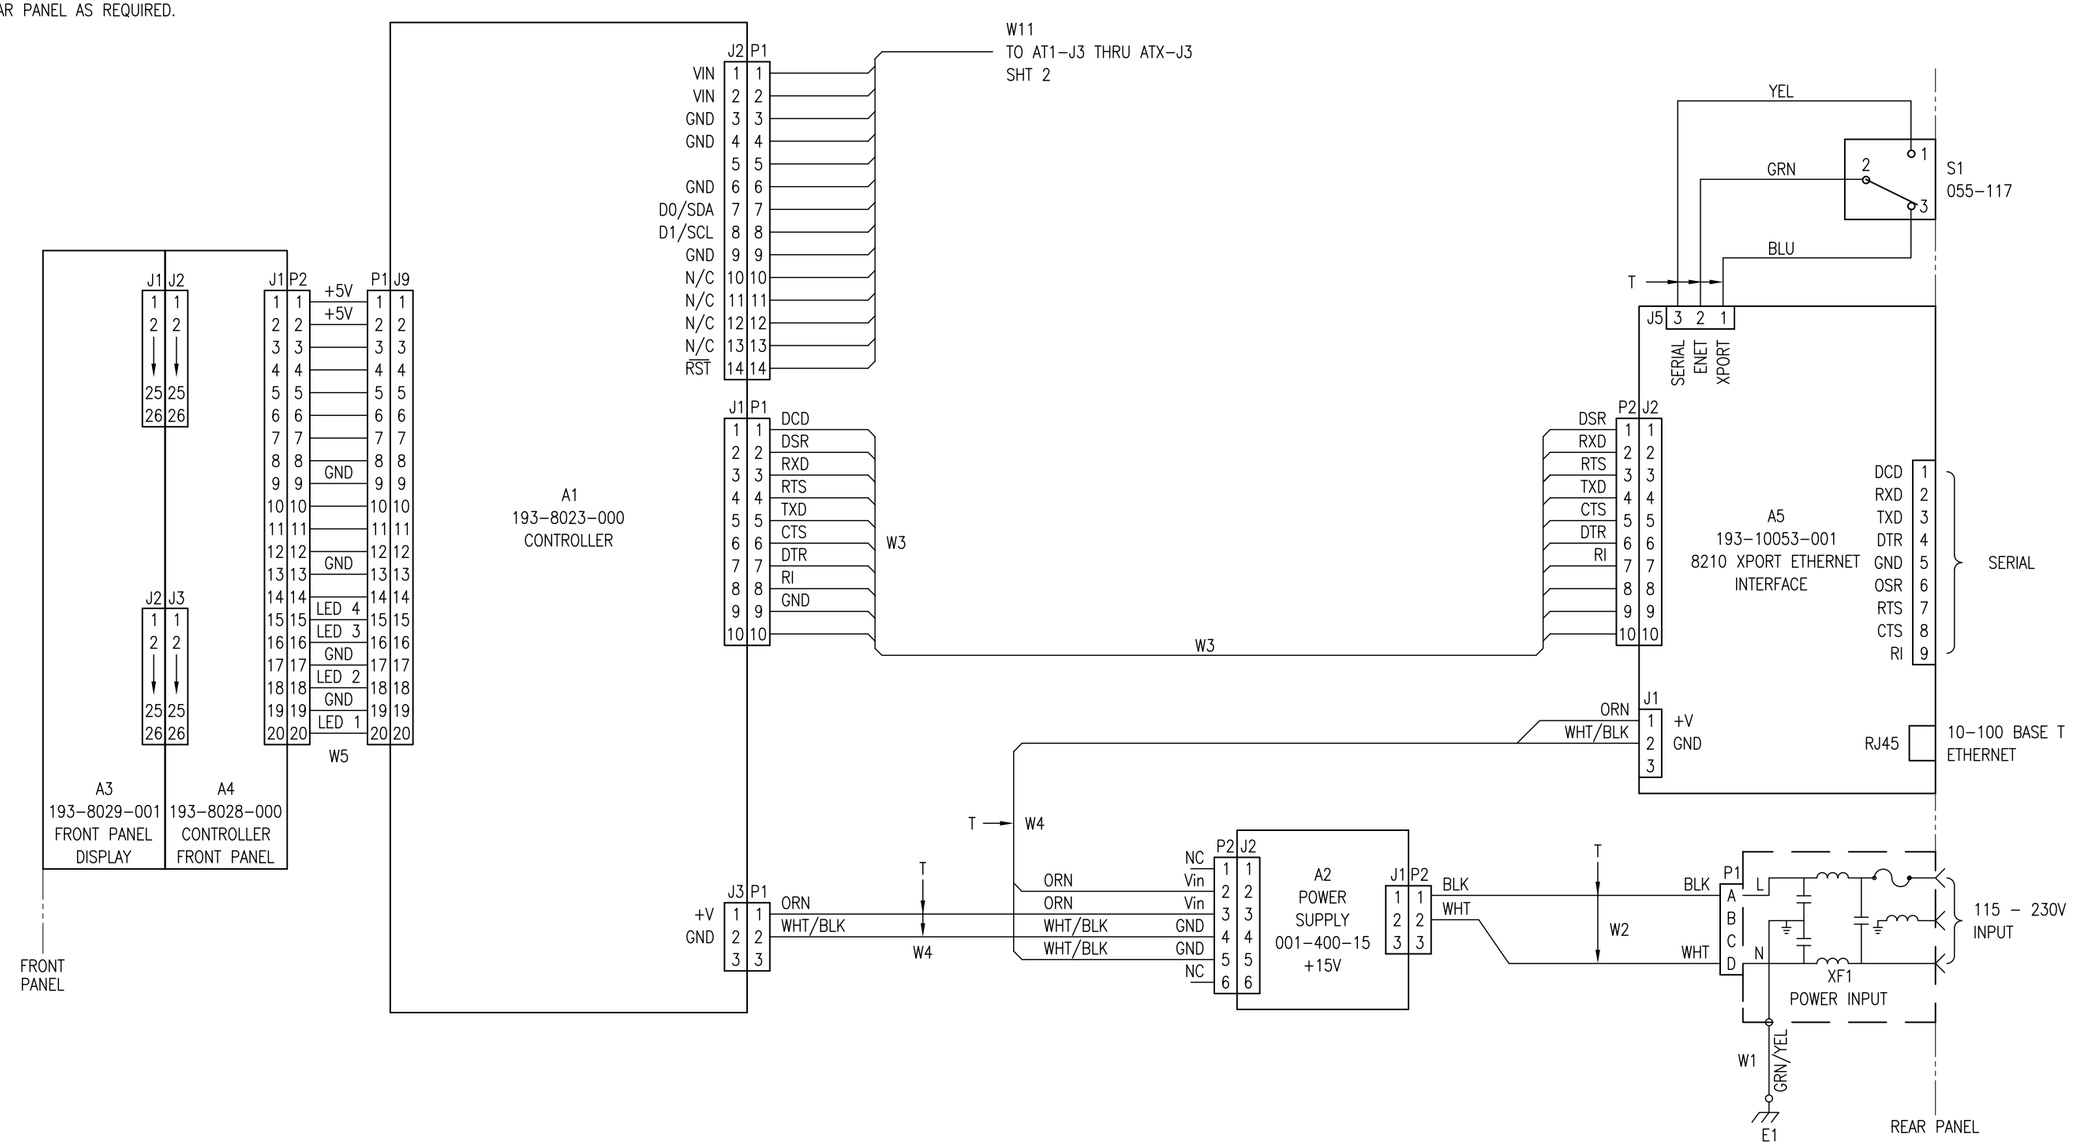

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.
PARTS LIST						

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

CONTRACT NO.

AEROFLEX WEINSCHEL

APPROVALS	DATE
DRAWN V. BETSIS	06/08
CHECKED A. HOPKINS	06/08
ENGR. W. KNILL	06/08
ISSUED	

WIRING DIAGRAM, ATTEN UNIT
8311 W/ETHERNET (+15V)

SIZE	CAGE:	DWG. NO.	REV.
D	93459	193–8141	B

SCALE NONE SHEET 1 OF 2

193–7307–2	8311–XXX–X–XN
NEXT ASSY	USED ON
APPLICATION	

MATERIAL
FINISH
DO NOT SCALE DRAWING

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
		SEE SHT 1 OF 1		

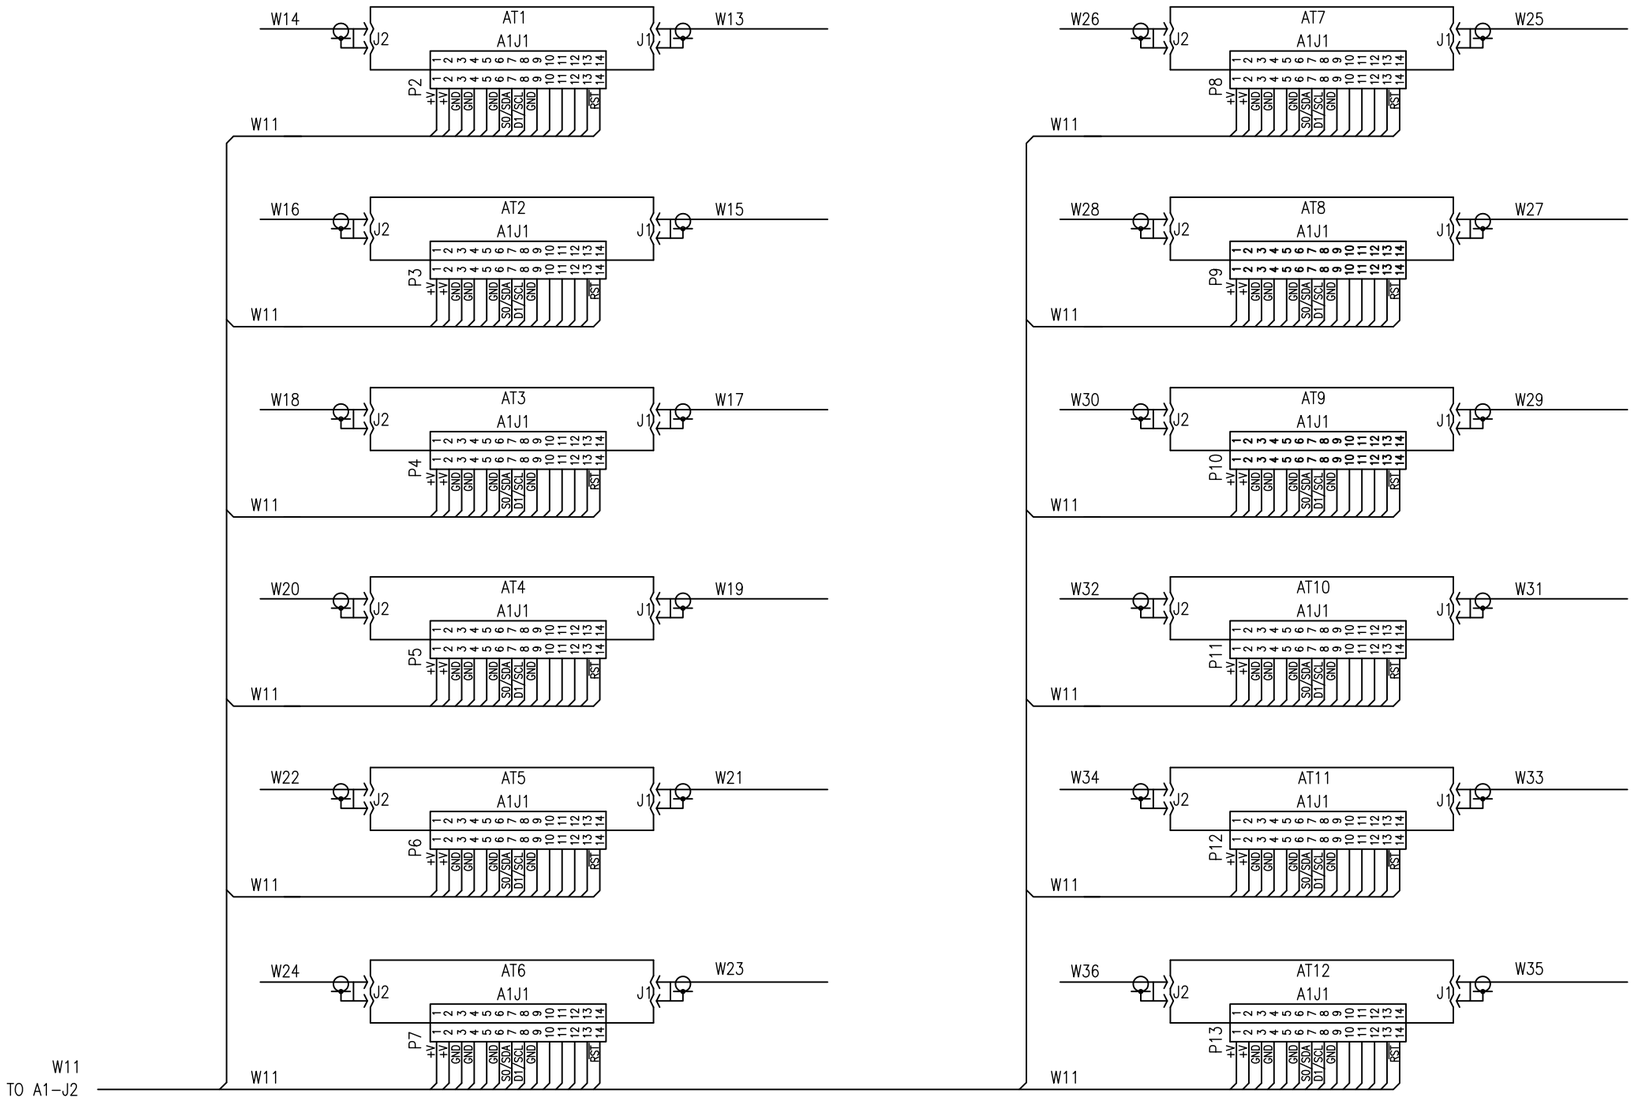

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.

PARTS LIST

193-7307-2	8311-XXX-X-XN
NEXT ASSY	USED ON
APPLICATION	

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL
FINISH
DO NOT SCALE DRAWING

CONTRACT NO.

APPROVALS	DATE
DRAWN	
CHECKED	
ENGR.	
ISSUED	

AEROFLEX WEINSCHEL

WIRING DIAGRAM, ATTEN UNIT MODEL 8311-352-X-XN

SIZE	CAGE:	DWG. NO.	REV.
D	93459	193-8141	B

SCALE NONE SHEET 2 OF 2

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS

ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 09-218 RS	DEC 09	

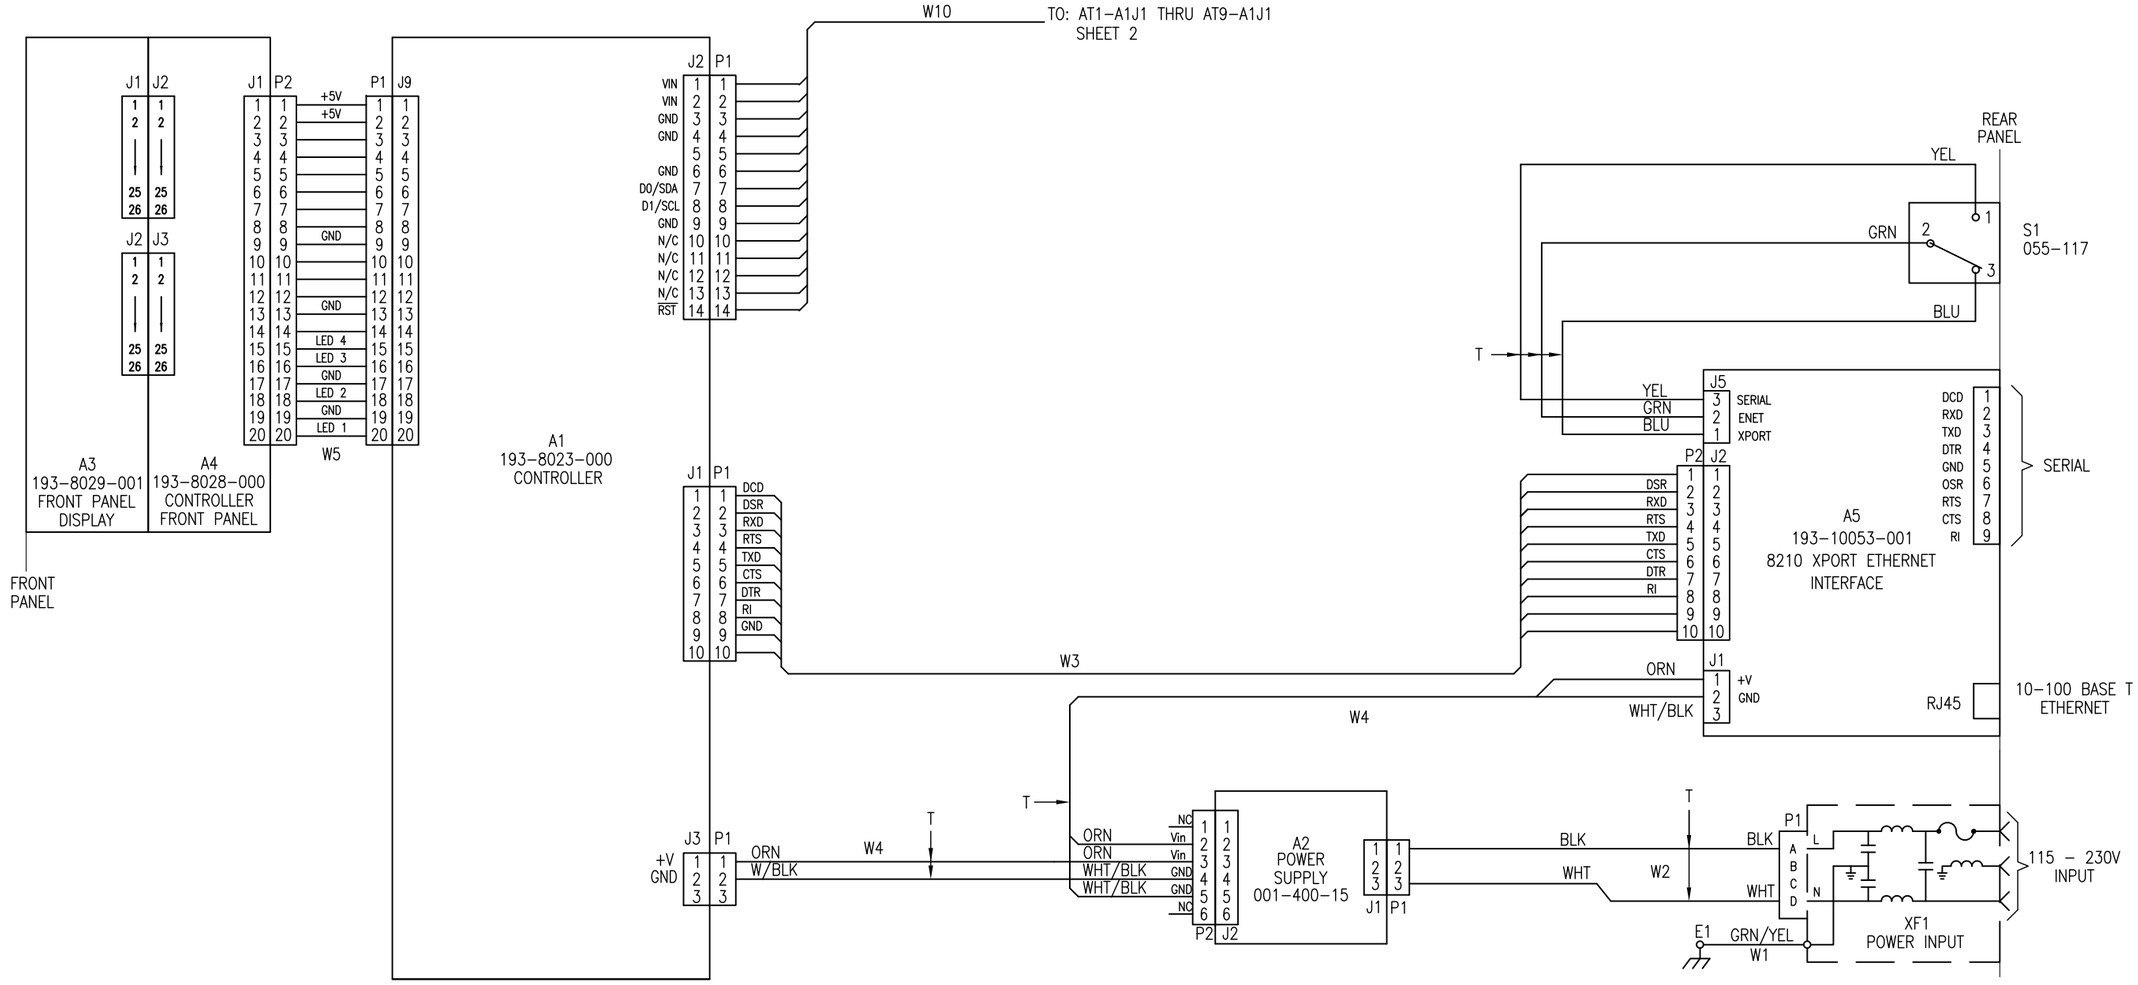

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.

PARTS LIST

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL

FINISH

DO NOT SCALE DRAWING

NEXT ASSY	USED ON
193-7307-9	8311-352-9-TN
APPLICATION	

CONTRACT NO.

APPROVALS	DATE
DRAWN R. SHOCK	2 DEC 09
CHECKED A. HOPKINS	DEC 09
ENGR. W. KNILL	DEC 09
ISSUED	

AEROFLEX WEINSCHEL

WIRING DIAGRAM, ATTEN UNIT 8311 W/ETHERNET (+15V)

SIZE	CAGE:	DWG. NO.	REV.
D	93459	193-8152	A

SCALE NONE SHEET 1 OF 2

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
		SEE SHT 1 OF 1		

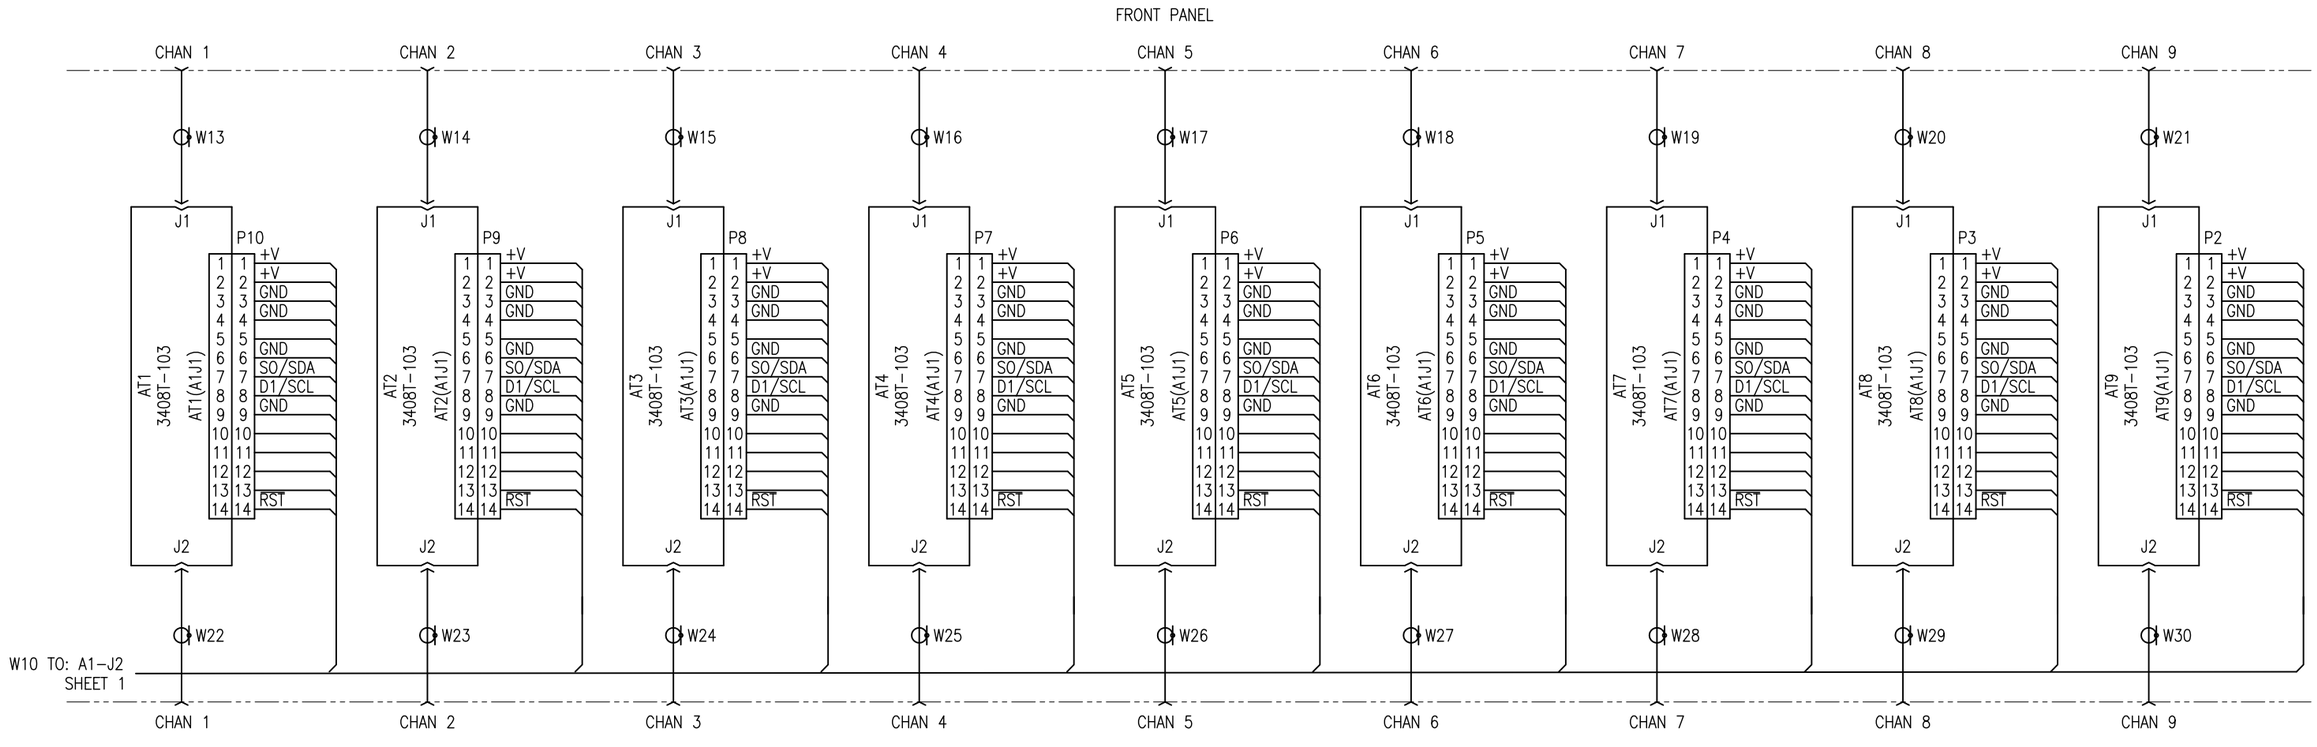

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.

PARTS LIST

193-7307-9	8311-352-9-TN
NEXT ASSY	USED ON
APPLICATION	

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL
FINISH
DO NOT SCALE DRAWING

CONTRACT NO.

APPROVALS	DATE
DRAWN	
CHECKED	
ENGR.	
ISSUED	

AEROFLEX WEINSCHEL

WIRING DIAGRAM, ATTEN UNIT MODEL 8311-352-9-TN

SIZE	CAGE:	DWG. NO.	REV.
D	93459	193-8152	A

SCALE NONE SHEET 2 OF 2

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 08-090 VB.	06/08	

NOTES:

1. POWER CORD, ITEM 24, SUPPLIED BUT NOT SHOWN
2. APPLY LOCTITE ON ALL HARDWARE AS REQUIRED
3. AFTER ASSEMBLY CONFIGURE AND TEST
4. APPLY LABEL SUPPLIED WITH ITEM 53 APPROX WHERE SHOWN
5. CAUTION WHEN MAITING PC BOARD CONNECTORS. MAKE SURE NO PINS ARE VISIBLE ON EITHER SIDE OF P1 CONNECTOR

WIRING CHART			
REF DES	FROM	TO	ITEM NO.
W1	XF1	CHASSIS GND	33
W2	XF1	A2-J1	6
W3	A1-J1	A5-J2	10
W4	A1-J3(P1) A2-J2 (P2-2) A2-J2 (P2-5)	A2-J2 (P2) A5-J1-1 (+V) A5-J1-2 (GND)	5
W5	A1-J9	A4-J1 FRONT PANEL	20

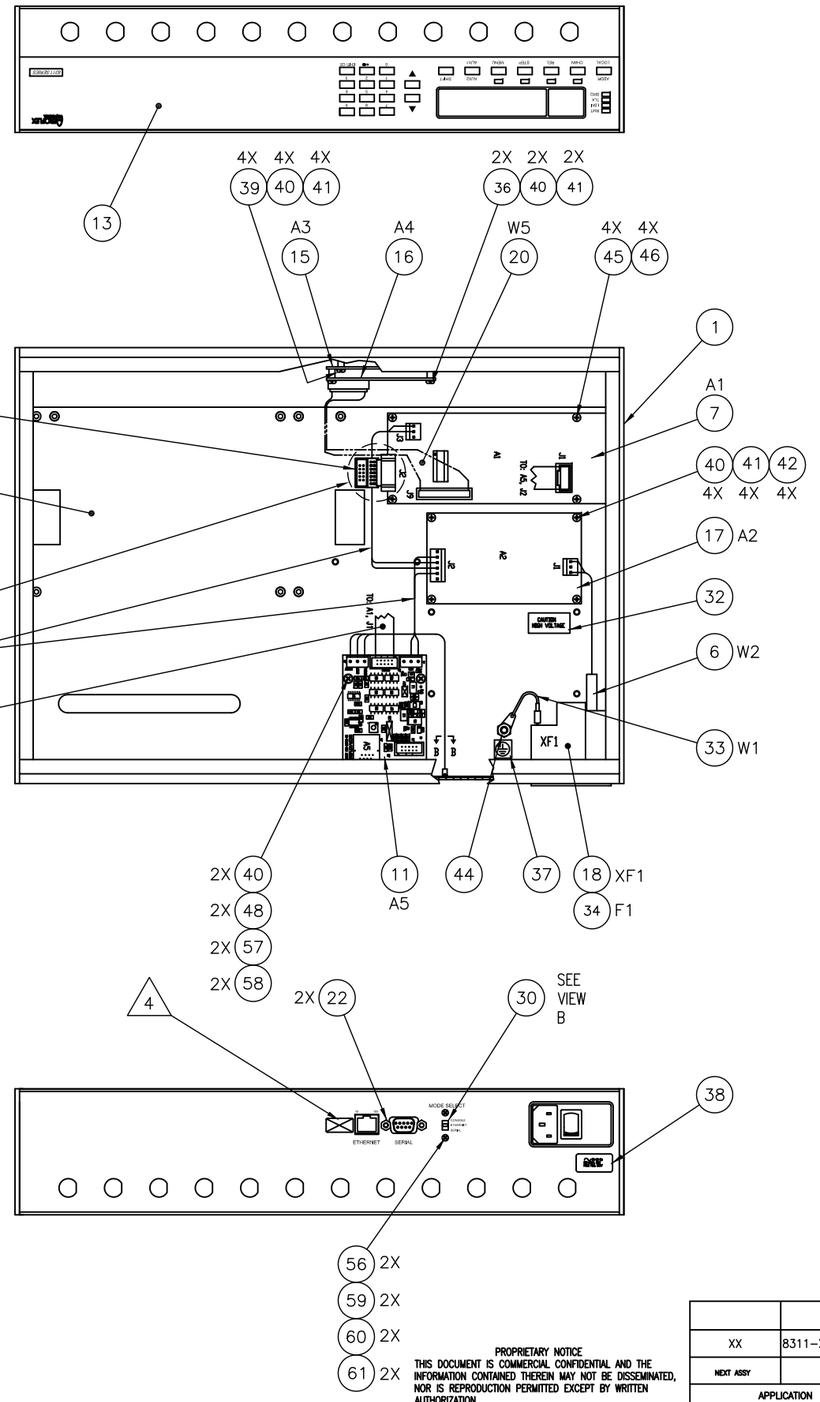

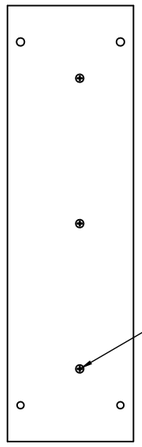

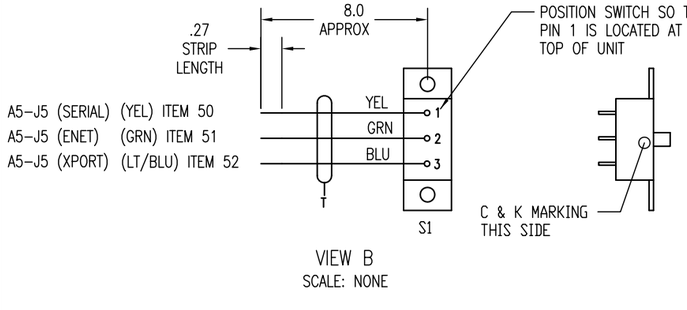

VIEW B
SCALE: NONE

SEE PARTS LIST SEE PL193-8138

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.
PARTS LIST						

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

XX	8311-XXX-X-XN
NEXT ASSY	USED ON
APPLICATION	

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL N/A
FINISH N/A
DO NOT SCALE DRAWING

CONTRACT NO.

APPROVALS	DATE
DRAWN V. BETSIS	06/08
CHECKED A. HOPKINS	06/08
ENGR. W. KNILL	06/08
ISSUED	

AEROFLEX WEINSCHEL

ASSY, ATTENUATOR
BASE UNIT, MODEL 8311 W/ETHERNET (+5V)

SIZE	CAGE:	DWG. NO.	REV.
D	93459	193-8138	A

SCALE 1:2 SHEET 1 OF 1

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 08-090 VB.	06/08	

NOTES:

1. POWER CORD, ITEM 24, SUPPLIED BUT NOT SHOWN
2. APPLY LOCTITE ON ALL HARDWARE AS REQUIRED
3. AFTER ASSEMBLY CONFIGURE AND TEST
4. APPLY LABEL SUPPLIED WITH ITEM 53 APPROX WHERE SHOWN

WIRING CHART			
REF DES	FROM	TO	ITEM NO.
W1	XF1	CHASSIS GND	33
W2	XF1	A2-J1	6
W3	A1-J1	A5-J2	10
W4	A1-J3(P1) A2-J2(P2-2) A2-J2(P2-5)	A2-J2(P2) A5-J1-1 (+V) A5-J1-2 (GND)	5
W5	A1-J9	A4-J1 FRONT PANEL	20

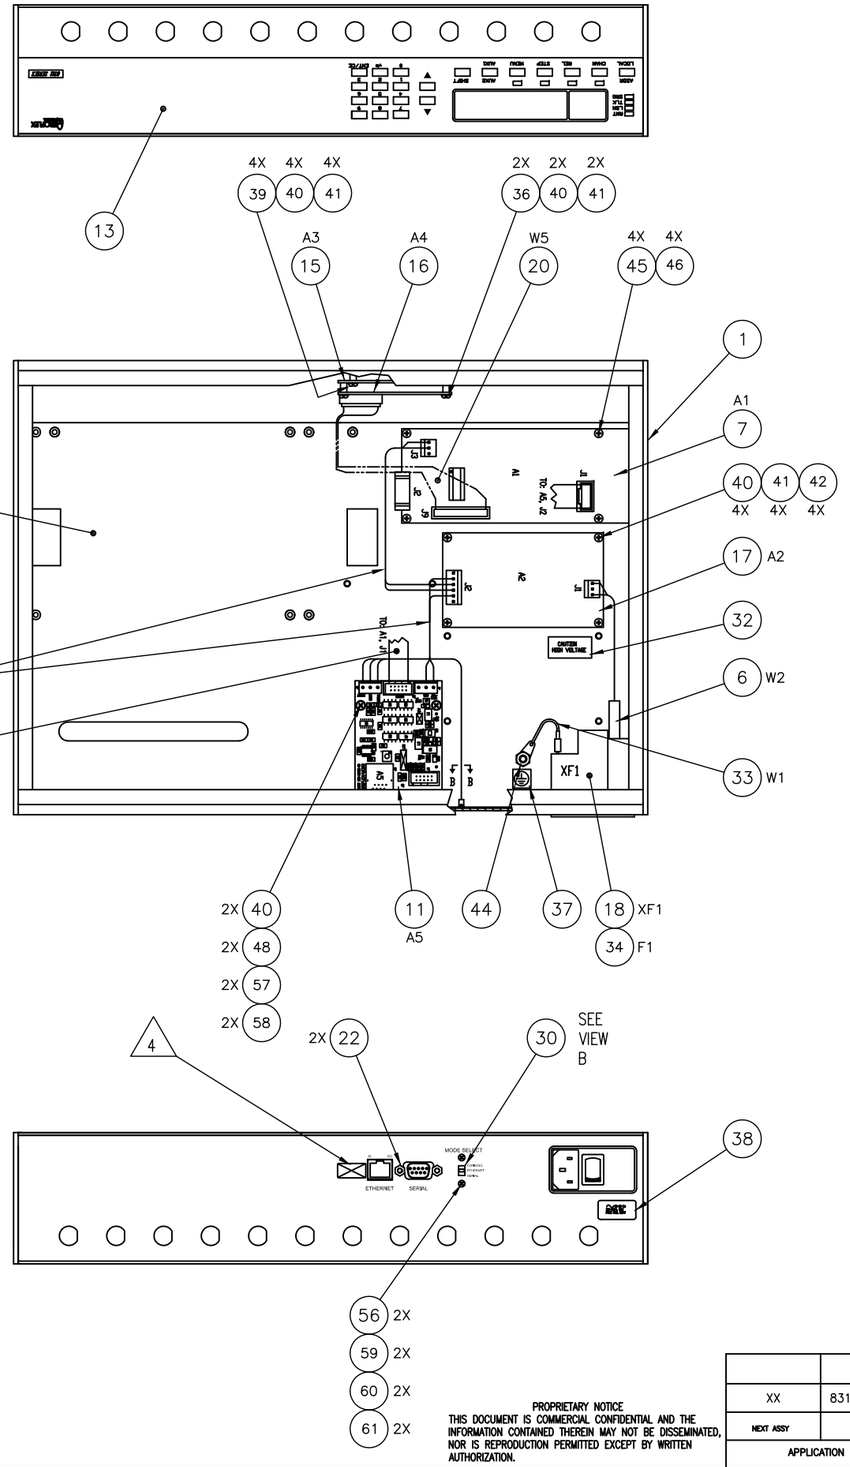

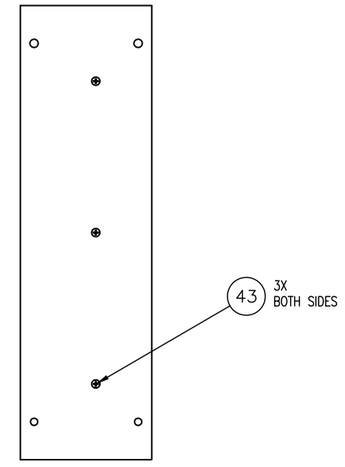

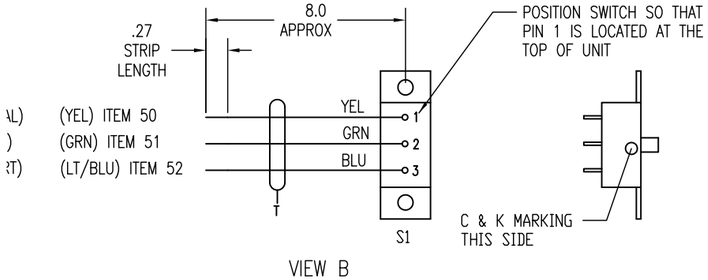

VIEW B

SEE PARTS LIST SEE PL193-8138-1

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.
PARTS LIST						

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL N/A

FINISH N/A

DO NOT SCALE DRAWING

CONTRACT NO.

APPROVALS	DATE
DRAWN V. BETSIS	06/08
CHECKED A. HOPKINS	06/08
ENGR. W. KNILL	06/08
ISSUED	

AEROFLEX WEINSCHEL

ASSY, ATTENUATOR
BASE UNIT, MODEL 8311
W/ETHERNET (+15V)

SIZE	CAGE:	DWG. NO.	REV.
D	93459	193-8138-1	A

SCALE 1:2 SHEET 1 OF 1

XX	8311-X-X-N
NEXT ASSY	USED ON
APPLICATION	

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS

ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 08-090 VB.	06/08	

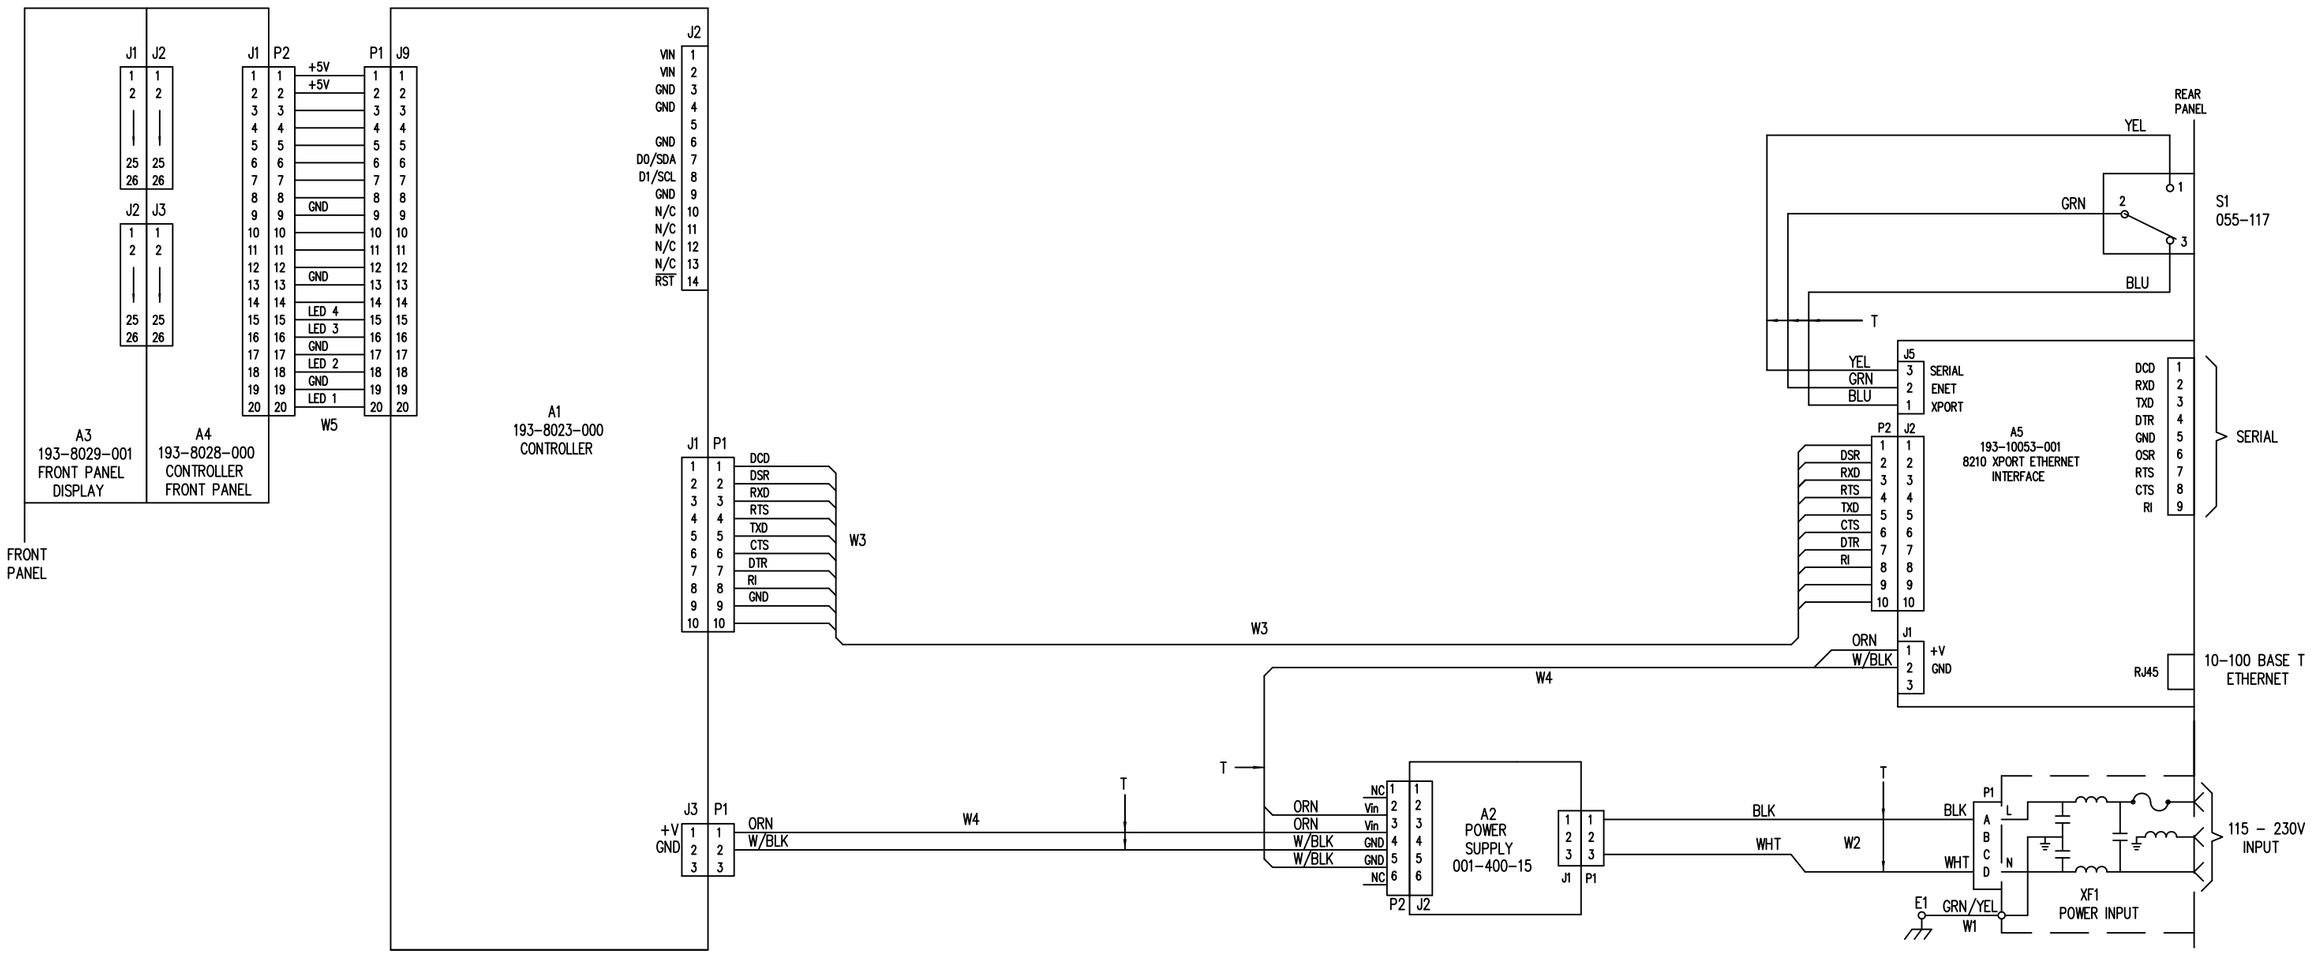

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.

PARTS LIST

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL

FINISH

DO NOT SCALE DRAWING

CONTRACT NO.

AEROFLEX WEINSCHEL

APPROVALS	DATE
DRAWN V. BETSIS	06/08
CHECKED A. HOPKINS	06/08
ENGR. W. KNILL	06/08
ISSUED	

WIRING DIAGRAM
ATTENUATOR BASE UNIT,
8311 W/ETHERNET (+15V)

SIZE	CAGE:	DWG. NO.	REV.
D	93459	193-8140	A

SCALE NONE SHEET 1 OF 1

NEXT ASSY	USED ON
193-8138-1	8311-XXX-X-XN

APPLICATION

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 09–102 GT	JUN 09	
	B	ERN 10–251 RS	AUG 10	

NOTES:
1. ALL DIMENSIONS GIVEN IN MM (INCHES)

SPECIFICATIONS:

BUS: IEEE 488, PROTOCOL PER 1EEE 488.2
RS232
OPERATIONAL TEMP: 0° TO +50°C
STORAGE TEMP: –55°C TO +75°C
WEIGHT: 12.5 LB MAX

SPECIFICATIONS							
MODEL NUMBER	ATTEN VALUE	FREQ RANGE	INSERTION LOSS	SWR	NO. CHANNEL	ATTEN TYPE	CONN TYPE	CONN LOCATION
8311–38–6–R–EN	63/1	dc TO 3000 MHz	5.25 dB MAX	1.5:1	6	3206T–1E	TYPE N/F	REAR
8311–38–6–RN	63/1	dc TO 2000 MHz	5.25 dB MAX	1.5:1	6	3206T–1	TYPE N/F	REAR

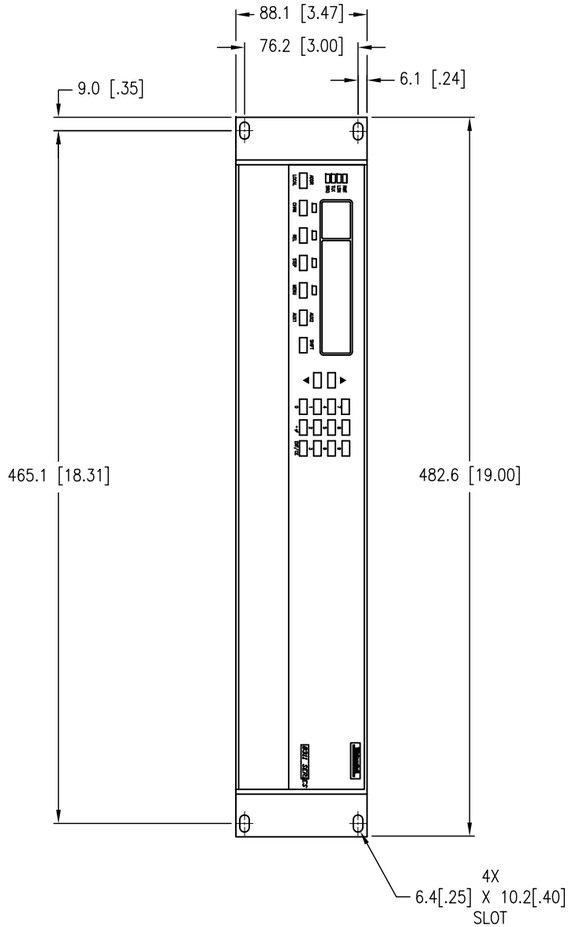

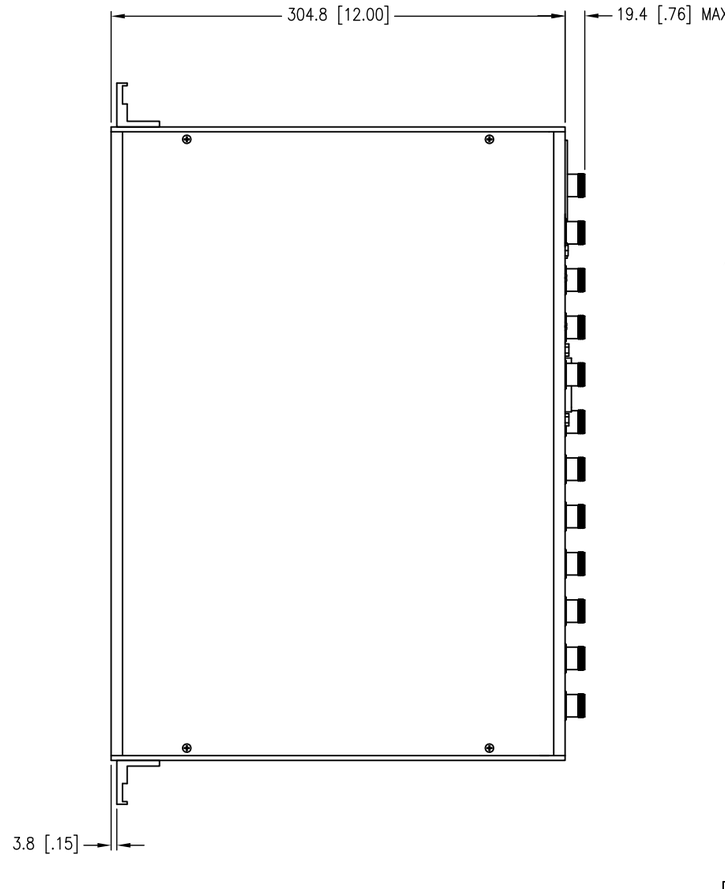

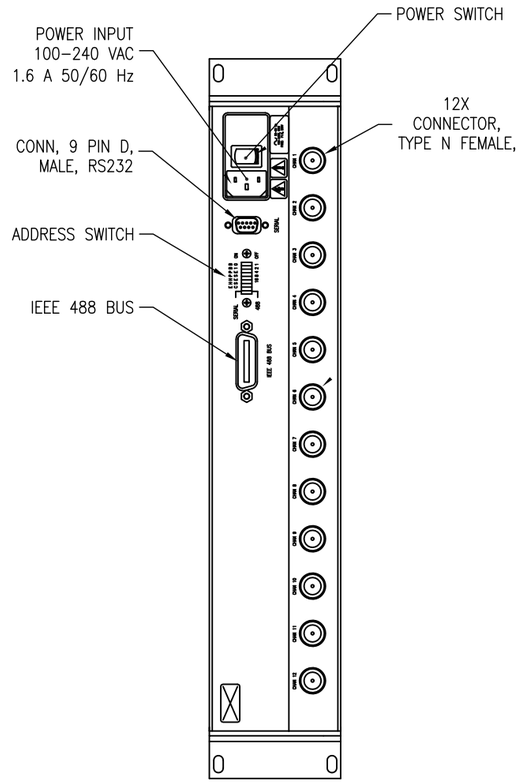

INTERFACE CONTROL DRAWING

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.
PARTS LIST						

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

.	8311
NEXT ASSY	USED ON
APPLICATION	

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL .
FINISH .
DO NOT SCALE DRAWING

CONTRACT NO.

APPROVALS	DATE
DRAWN G. THOMAS	4 JUN 09
CHECKED A. HOPKINS	JUN 09
ENGR. B. KNILL	JUN 09
ISSUED	

AEROFLEX WEINSCHEL

ICD, MULTI–CHANNEL ATTENUATOR
MODEL 8311–38–6–R–EN
MODEL 8311–38–6–RN

SIZE	CAGE:	DWG. NO.	REV.
D	93459	089–4157	B

SCALE 1:2 SHEET 1 OF 1

AUTOCAD V.2007

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
		SEE SH 1		

NOTES: UNLESS OTHERWISE SPECIFIED.

1. ALL DIMENSIONS GIVEN IN MM [INCHES].

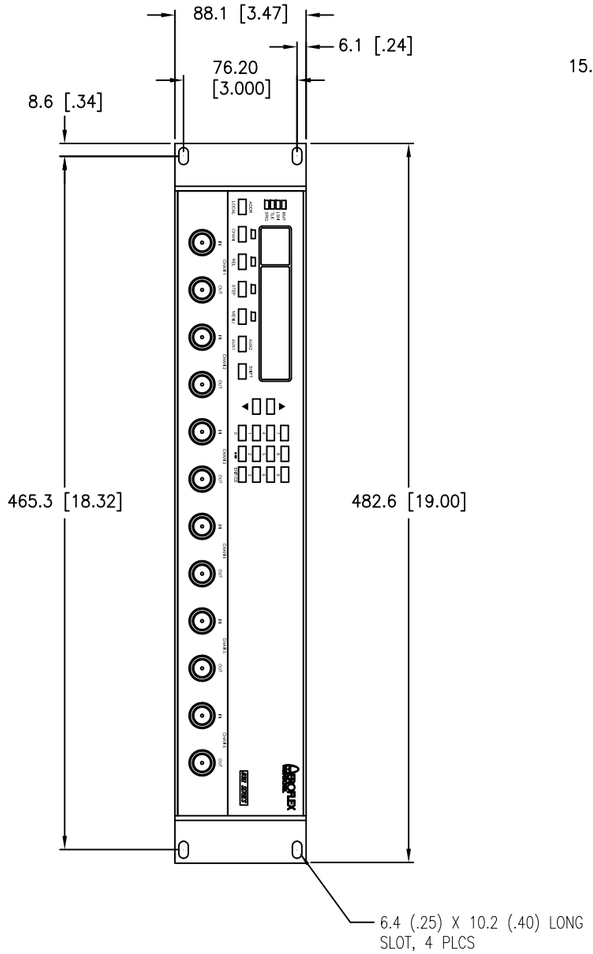

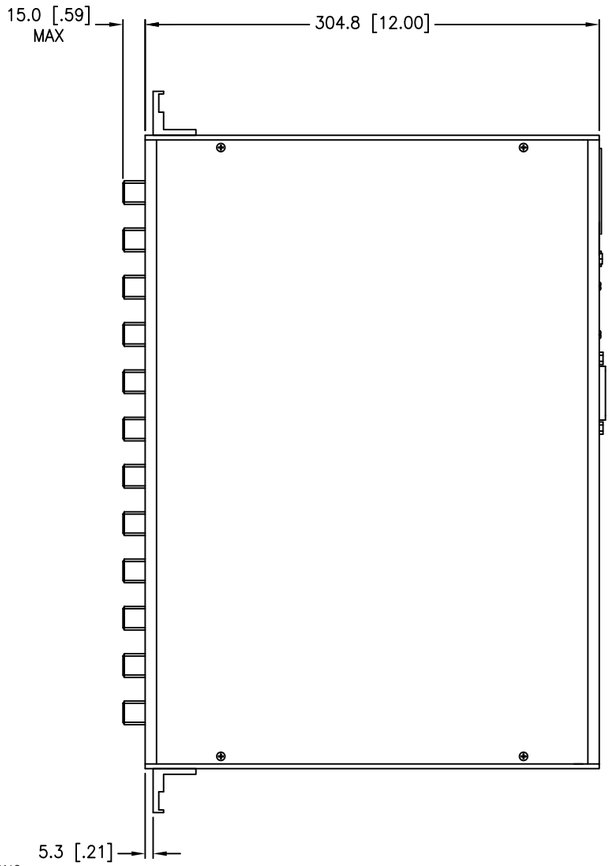

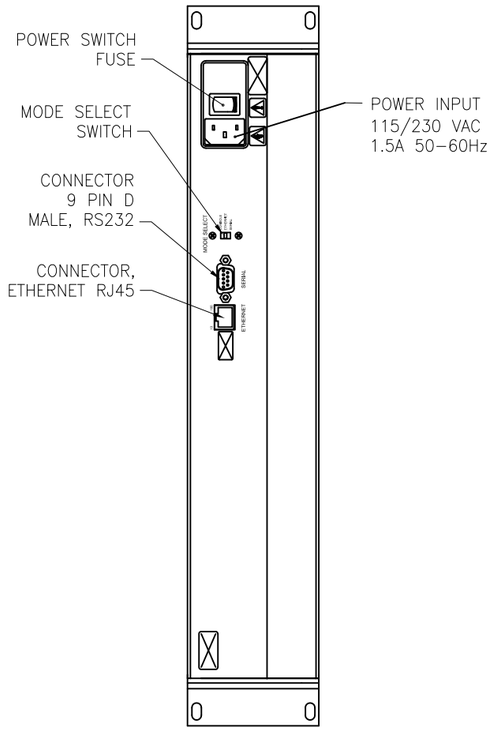

SPECIFICATIONS:

BUS: IEEE 488, PROTOCOL PER 1EEE 488.2
RS232
OPERATIONAL TEMP: 0° TO +50°C
STORAGE TEMP: −55°C TO +75°C
WEIGHT: 12.5 LB MAX

MODEL NO.	ATTEN VALUE	FREQ RANGE	INSERTION LOSS	SWR	NO. CHANNEL	ATTEN TYPE	CONN TYPE	CONN LOCATION
8311-38-6-FN	63/1	dc TO 2000 MHz	5.25 dB MAX	1.5:1	6	3206T-1	TYPE N/F	FRONT

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

NEXT ASSY	USED ON
	8311
APPLICATION	

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .005 ANGLES ± 1/2°

MATERIAL .

FINISH .

DO NOT SCALE DRAWING

CONTRACT NO.		
APPROVALS	DATE	
DRAWN G. THOMAS	4 JUN 09	
CHECKED A. HOPKINS	JUN 09	
ENGR. B. KNILL	JUN 09	
ISSUED		

INTERFACE CONTROL DRAWING

AEROFLEX WEINSCHEL

ICD, MULTI-CHANNEL ATTENUATOR
MODEL 8311-38-6-FN

SIZE	CAGE:	DWG. NO.	REV.
D	93459	089-4157	A

SCALE 1:1 SHEET 2 OF 2

AUTOCAD V.2007

DWG. NO.	SH 1	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 08-128	08/08	

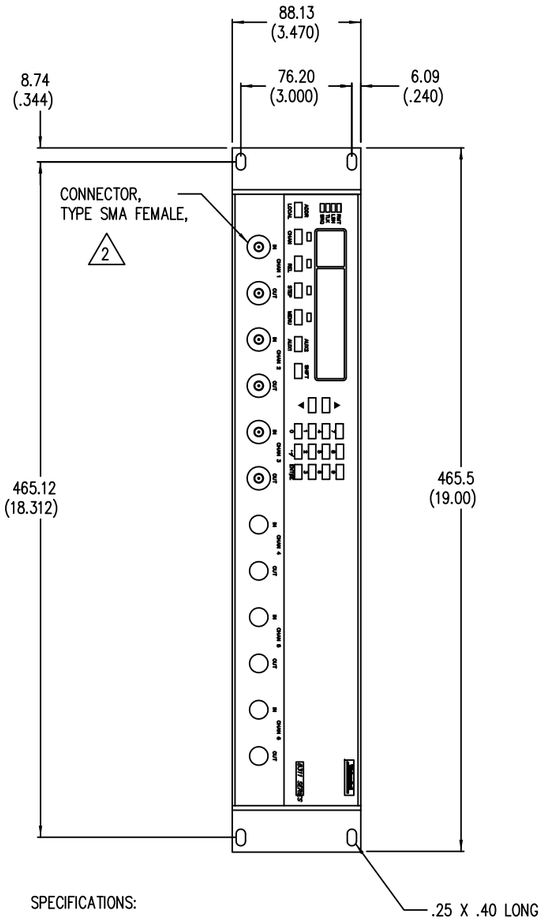

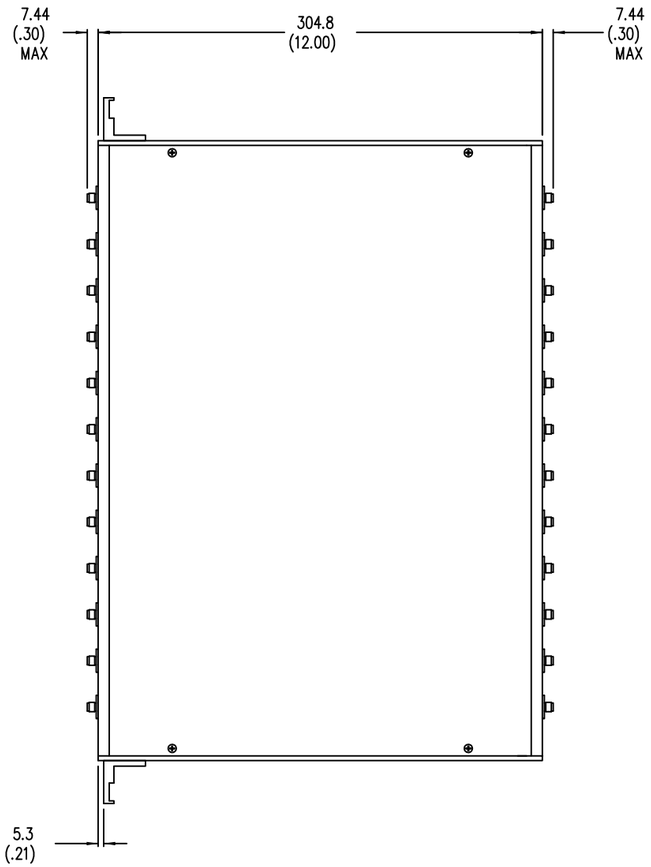

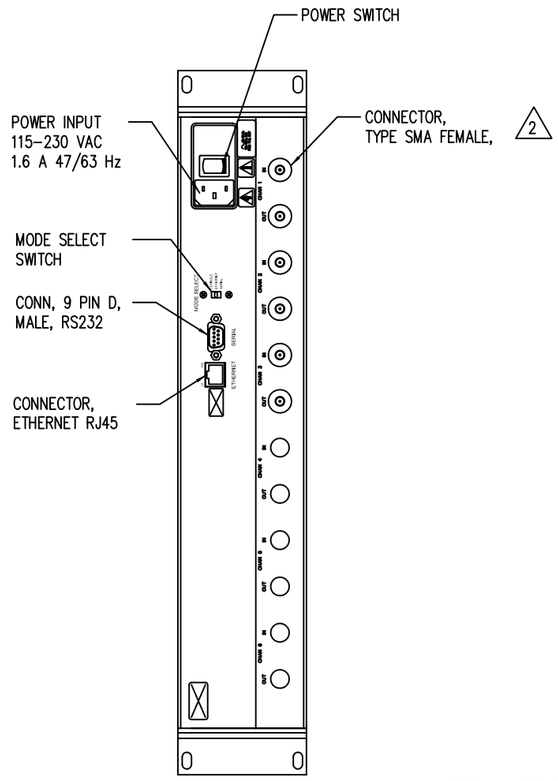

SPECIFICATIONS:

OPERATIONAL TEMP: 0° TO +50°C
STORAGE TEMP: −55°C TO +75°C
WEIGHT: 12.5 LB MAX

MODEL NO.	ATTEN VALUE	FREQ RANGE	INSERTION LOSS	SWR	NO. CHANNEL	ATTEN TYPE (1)	CONN TYPE	CONN LOCATION
8311-202-2-FN	121/1	DC-18 GHz	5.25 MAX	1.95	2	150T-11 + 150T-110	SMA/F	FRONT
8311-202-2-RN	121/1	DC-18 GHz	5.25 MAX	1.95	2	150T-11 + 150T-110	SMA/F	REAR
8311-202-3-FN	121/1	DC-18 GHz	5.25 MAX	1.95	3	150T-11 + 150T-110	SMA/F	FRONT
8311-202-3-RN	121/1	DC-18 GHz	5.25 MAX	1.95	3	150T-11 + 150T-110	SMA/F	REAR

(1) SEE ATTENUATOR INTERFACE CONTROL DRAWING FOR RF SPECIFICATIONS

NOTES: UNLESS OTHERWISE SPECIFIED.

1. ALL DIMENSIONS GIVEN IN MM (INCHES)

2 CONNECTORS INSTALLED FRONT OR REAR AS REQUIRED.

PROPRIETARY NOTICE

THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

INTERFACE CONTROL DRAWING

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.

PARTS LIST

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL

FINISH

DO NOT SCALE DRAWING

NEXT ASSY	USED ON
APPLICATION	

CONTRACT NO.

APPROVALS	DATE
DRAWN M. TYSON	8/08
CHECKED HOPKINS	8/08
ENGR. KNILL	8/08
ISSUED	

AEROFLEX WEINSCHEL

ICD, MULTI-CHANNEL ATTENUATOR

SIZE	FSCM NO.	DWG. NO.	REV.
D	93459	089-4090	A

SCALE 1/2 SHEET 1 OF 1

DWG. NO.	SH	REV.

REVISIONS

ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 08-091 VB.	06/08	

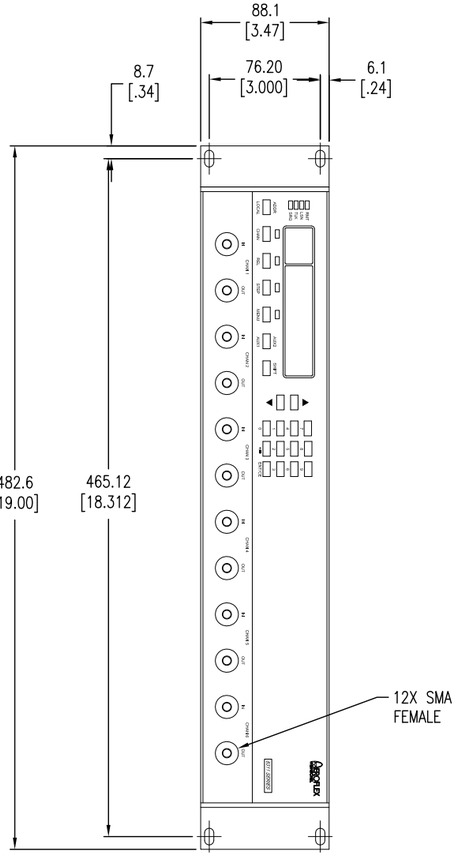

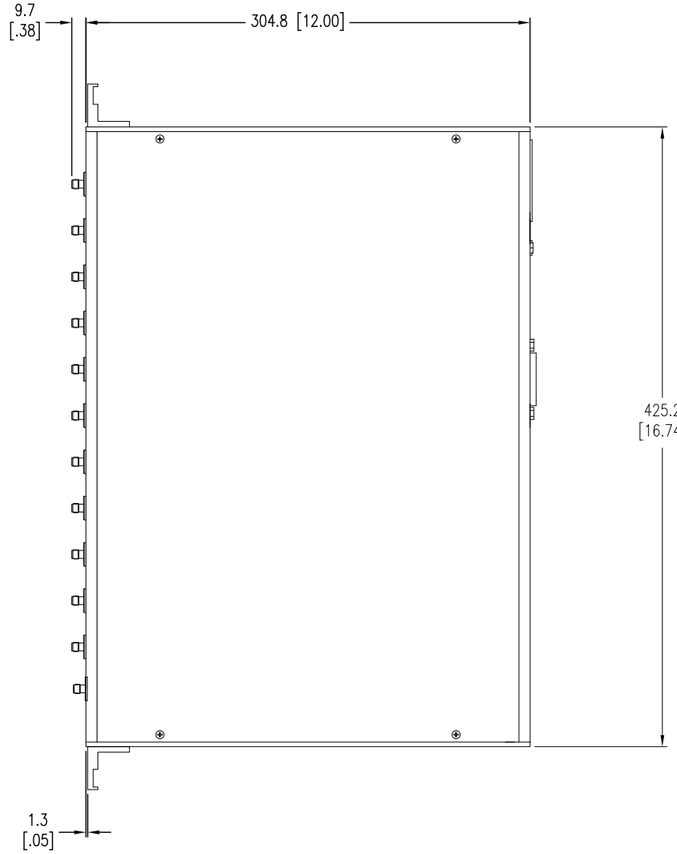

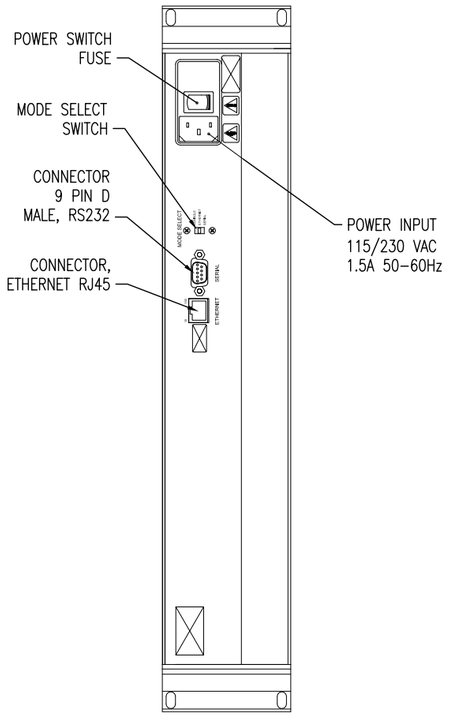

MODEL NUMBER	ATTEN VALUE	FREQ RANGE	INSERTION LOSS	SWR	NO. OF CHAN	ATTEN TYPE (1)	CONN TYPE	CONN LOCATION
8311-352-6-FN	103/1	DC - 6.0 GHz	6.0dB	1.55	6	3408T-103	SMA/F	FRONT

(1) SEE ATTENUATOR INTERFACE CONTROL DRAWING FOR RF SPECIFICATIONS

NOTES:
1. ALL DIMENSIONS GIVEN IN MM [INCHES]

INTERFACE CONTROL DRAWING

ITEM NO.	ZONE	MATERIAL SPECIFICATION	NOMENCLATURE OR DESCRIPTION	PART OR IDENTIFYING NO.	FSCM NO.	QTY REQD

PARTS LIST

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS XX ± .01 XXX ± .003 ANGLES ± 1/2°

MATERIAL .

FINISH .

DO NOT SCALE DRAWING

CONTRACT NO.

APPROVALS		DATE
DRAWN	V. BETSIS	06/08
CHECKED	A. HOPKINS	06/08
ENGR.	W. KNILL	06/08
ISSUED		

Aeroflex / Weinschel

ICD, ATTEN UNIT
MODEL 8311 SERIES
(6 CHANNEL)

SIZE	FSCM NO.	DWG. NO.	REV.
D	93459	089-4073	C

SCALE 1 : 2 SHEET 1 OF 1

NEXT ASSY	USED ON
193-XXXX-X	8311-352-6-FN

APPLICATION

PROPRIETARY NOTICE

THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

DWG. NO.	SH	REV.

REVISIONS				
ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 09-218 RS	DEC 09	

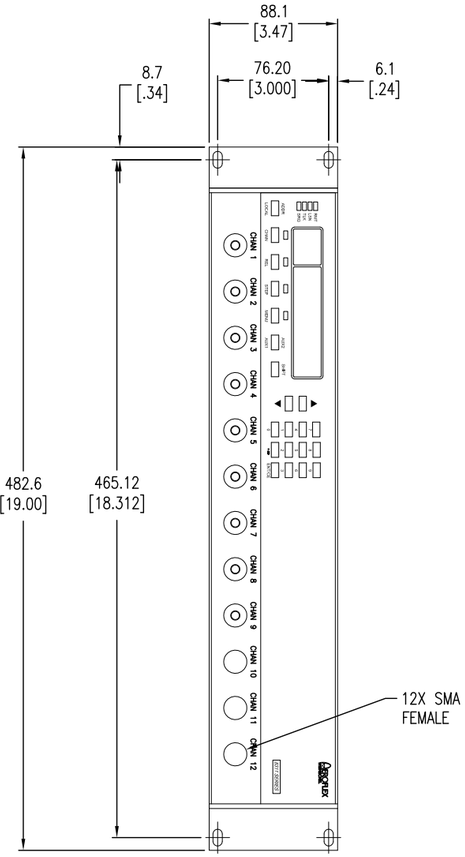

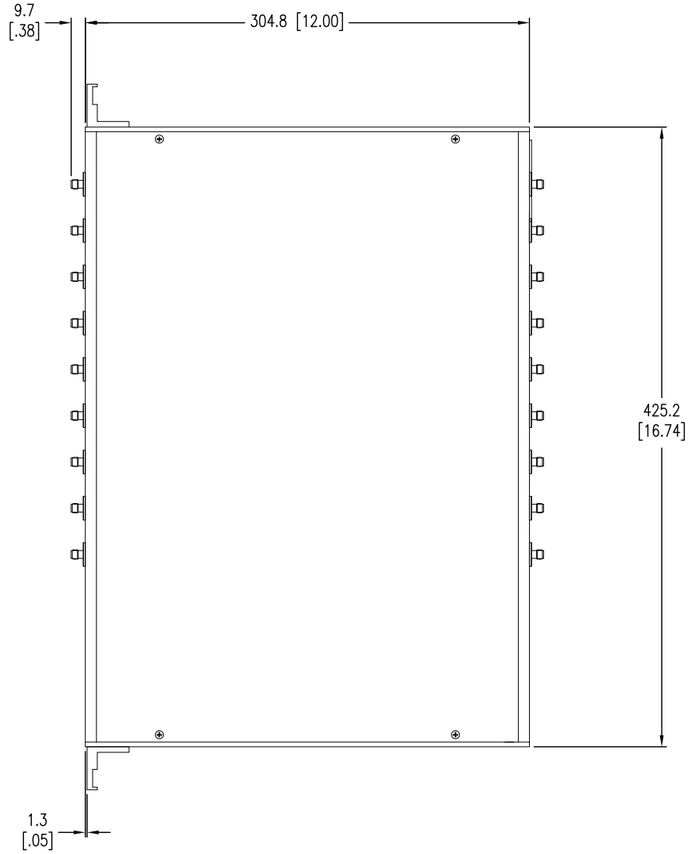

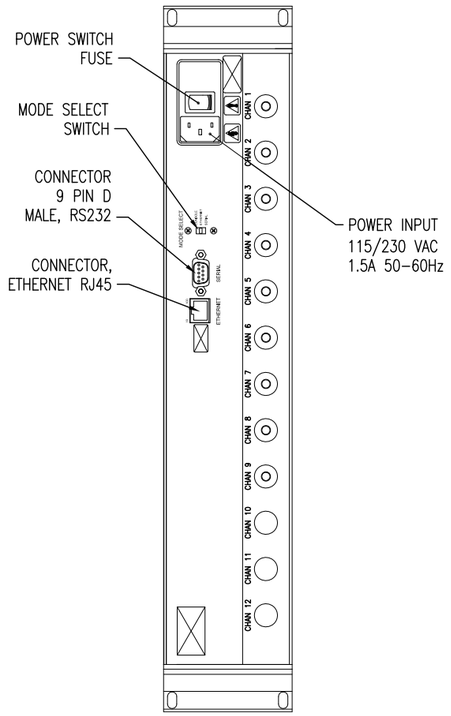

MODEL NUMBER	ATTEN VALUE	FREQ RANGE	INSERTION LOSS	SWR	NO. OF CHAN	ATTEN TYPE (1)	CONN TYPE	CONN LOCATION
8311-352-9-TN	103/1	DC – 6.0 GHz	6.0dB	1.55	9	3408T-103	SMA/F	FRONT/REAR

(1) SEE ATTENUATOR INTERFACE CONTROL DRAWING FOR RF SPECIFICATIONS

NOTES:
1. ALL DIMENSIONS GIVEN IN MM [INCHES]

INTERFACE CONTROL DRAWING

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.
PARTS LIST						

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

193-7307-9	8311-352-9-TN
NEXT ASSY	USED ON
APPLICATION	

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL .
FINISH .
DO NOT SCALE DRAWING

CONTRACT NO.

APPROVALS	DATE
DRAWN V. BETSIS	2 DEC 09
CHECKED A. HOPKINS	DEC 09
ENGR. W. KNILL	DEC 09
ISSUED	

Aeroflex / Weinschel

ICD, ATTEN UNIT MODEL 8311 SERIES (9 CHANNEL)

SIZE	FSCM NO.	DWG. NO.	REV.
D	93459	089-4193	A

SCALE 1 : 2 SHEET 1 OF 1

DWG. NO.	SH	REV.

REVISIONS

ZONE	REV.	DESCRIPTION	DATE	APPROVED
	A	ERN 10-180 RS	OCT 10	

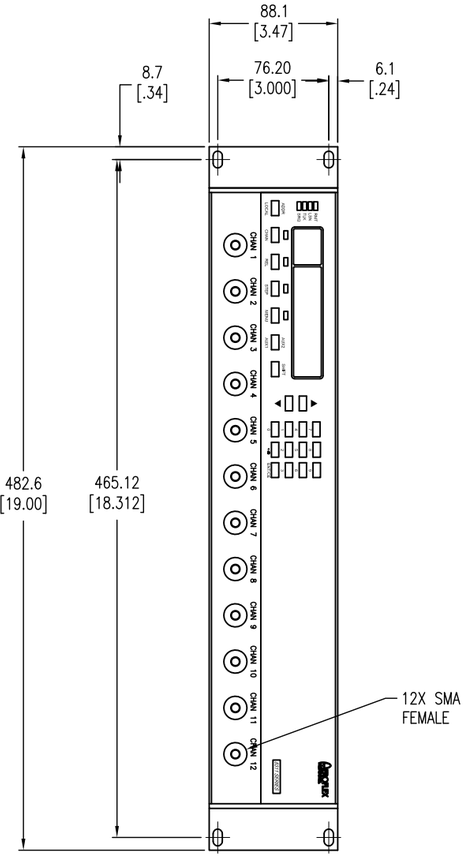

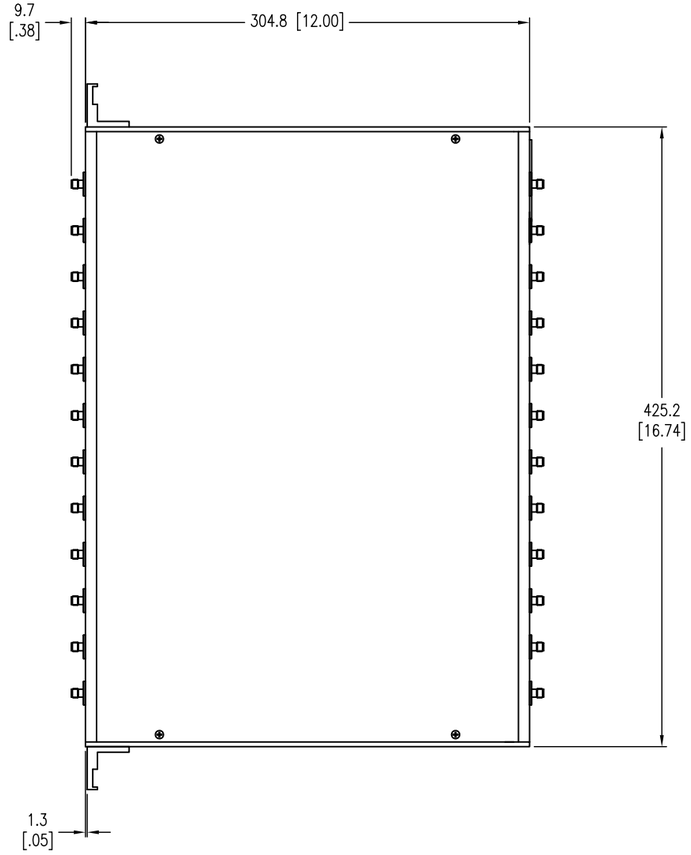

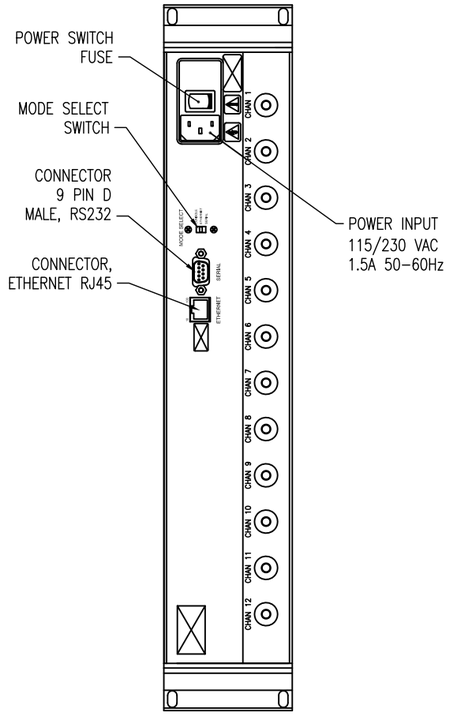

MODEL NUMBER	ATTEN VALUE	FREQ RANGE	INSERTION LOSS	SWR	NO. OF CHAN	ATTEN TYPE (1)	CONN TYPE	CONN LOCATION
8311-352-12-TN	103/1	DC – 6.0 GHz	6.0dB	1.55	12	3408T-103	SMA/F	FRONT/REAR

(1) SEE ATTENUATOR INTERFACE CONTROL DRAWING FOR RF SPECIFICATIONS

NOTES:
1. ALL DIMENSIONS GIVEN IN MM [INCHES]

INTERFACE CONTROL DRAWING

QTY REQD	FSCM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	ZONE	ITEM NO.

PARTS LIST

PROPRIETARY NOTICE
THIS DOCUMENT IS COMMERCIAL CONFIDENTIAL AND THE INFORMATION CONTAINED THEREIN MAY NOT BE DISSEMINATED, NOR IS REPRODUCTION PERMITTED EXCEPT BY WRITTEN AUTHORIZATION.

193-7307-13	8311-352-9-TN
NEXT ASSY	USED ON
APPLICATION	

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS ± 1/64 DECIMALS .XX ± .01 .XXX ± .003 ANGLES ± 1/2°

MATERIAL .
FINISH .
DO NOT SCALE DRAWING

CONTRACT NO.

APPROVALS	DATE
DRAWN R. SHOCK	20 OCT 10
CHECKED A. HOPKINS	OCT 10
ENGR. B. FORRESTEL	OCT 10
ISSUED	

Aeroflex / Weinschel

ICD, ATTEN UNIT
MODEL 8311 SERIES
(12 CHANNEL)

SIZE	FSCM NO.	DWG. NO.	REV.
D	93459	089-4255	A

SCALE 1 : 2 SHEET 1 OF 1

APPENDIX A
CARE AND HANDLING OF MICROWAVE COAXIAL CABLE ASSEMBLIES

A-1 CARE AND HANDLING OF ASSEMBLIES.

To ensure accurate measurements and optimal performance of Weinschel products, the microwave coaxial cable assemblies used in system and test setups must be properly used and maintained. Proper connections, routine inspection of all cables, and cleaning of the connectors are extremely important procedures which can prolong the longevity and accuracy of equipment.

A-2 CABLE INSPECTION.

Routinely check external cables for signs of cracked insulation, dents, twists, flattening, signs of jacket abrasion, or other signs of abuse. Wrinkles in the jacket indicate that the minimum bend radius has been exceeded. Most often, this occurs near the marker tubes and connectors.

Also inspect the connector interfaces for the following:

- Bent pins (male).
- Bent or missing tines (female).
- Worn or chipped plating.
- Damaged or displaced dielectric inserts.
- Thread damage.
- Folded or mushroomed outer interface rims.
- Mushroomed pin shoulders (male) or tine ends (female).
- Score lines on pins and outer interface rims visible to the unaided eye.
- Recessed or protruding pins.

It is advisable to clean the connectors prior to inspection to make subtle damage more apparent. If any of the above is noted, replace the assembly before its further use results in equipment damage. Also inspect the mating connectors for similar damage.

Inspect the connector interface for signs of debris. Debris may be in the form of:

- Plating chips or other metal particles.
- Dust or dirt.
- Oily films.
- Other miscellaneous foreign particles.

If signs of debris are present, clean the connector interface as directed in Paragraph A-6.

A-3 MAKING INITIAL CONNECTIONS.

Exercise caution when mating cables. Poor connections lead to poor system performance. They can also damage not only the cable assembly, but more significantly, front or rear panel connectors on the equipment itself which may be more difficult to repair.

A-3.1 ALIGNING CONNECTORS. Align the center lines of two connectors before actual mating. Male retaining nuts contain a small amount of necessary play which may make it possible to mate the threads without the pins being properly aligned. Pin misalignment can damage pins and dielectric inserts.

A-3.2 MATING CONNECTORS. Gently mate the connectors by hand, taking care not to force the coupling nut at the slightest resistance. It is often possible to feel whether or not the pins are mated. If the coupling nut is difficult to turn, either the pins are not mated, the coupling nut is cross-threaded, or one of the connectors has been damaged by excess torque.

Never hold a male connector coupling nut stationary while screwing a female connector into it. This rotation can erode the plating and damage both the outer interface rim as well as the pin. If the pins become locked, serious damage can result to both the equipment and the cable assembly.

A-4 ENSURING PROPER CONNECTOR TORQUE.

A-4.1 OVERTORQUING. Once connectors have been properly mated, apply only the proper amount of torque. Overtorquing damages both connectors involved. Also, a connector which has been damaged by overtorquing, in turn, damages every connector to which it is subsequently mated. It usually leads to poor system performance as well. Overtorque can cause:

- Bent pins.
- Recessed or protruding pins.
- Recessed or protruding dielectrics.
- Chipped plating.
- Damaged coupling threads.
- Coupling nut retaining ring damage.
- Mushroomed outer interface shells.
- Mushroomed pin shoulders.

A-4.2 HEX-NUT TYPES. To mate a connector of the hex-nut type, always use a torque wrench set to the correct torque value. Tighten the connector slowly until the wrench snaps. Tightening too quickly can cause the wrench to exceed its set limit. Do not snap the wrench more than once as this also causes overtorque.

A-4.3 KNURLED NUTS. Tighten connectors with knurled nuts by hand. If this does not provide sufficient tightness use a hex-nut connector and torque wrench instead. Never use pliers to tighten a connector. Table A-1 recommends torque specifications for the various types of connectors.

Table A-1. Recommended Torque Values

Connector	Recommended Torque
GPC-7 (7mm) w/hex nut	14 in/lbs ± 1 in/lbs
Type N w/hex nut	14 in/lbs ± 1 in/lbs
SMA, 2.92mm, 3.5mm 2.4mm, WPM, WPM-3 WPM-4	7.5 in/lbs ± 0.5 in/lbs
Type N & TNC (knurled)	Hand-tight
BNC (knurled)	Hand-tight

A-5 PROPER CABLE HANDLING.

Never exceed the minimum bend radius specified for a cable. Guard against tight bends at the end of connector strain relief tubing, or at the ends of marker tubing where they may be less noticeable. Although cable bend may seem slight, the actual radius of the bend at the point of angular departure may be far smaller than the acceptable radius.

Never pinch, crush or drop objects on cable assemblies. Also, do not drag a cable over sharp edges as this will pinch it and cause it to exceed the minimum bend radius.

Never use a cable assembly to pull a piece of equipment. Cables and connectors are not designed to support or move equipment.

A-5.1 SECURING CABLES. Use toothed, rubber-lined "P-clamps" to hold cables in place. If it is necessary to use tie-wraps, use the widest possible wrap and the lowest setting on the gun to ensure the minimum pressure on the cable.

A-5.2 STORING CABLES. When storing cables, minimize cable "set" by coiling them in large diameters (1 or 2 feet). Unroll the cable properly when it is ready to be used; do not pull the loops out hastily. Similarly, re-roll them when storing them away again.

A-6 CLEANING CONNECTOR INTERFACES.

Use the following guidelines in cleaning connector interfaces:

a. Do not use chlorinated solvents including common tap water. These solvents are extremely penetrating and sometimes ruin otherwise good devices and assemblies.

b. Moisten a cotton swab with isopropyl alcohol. Roll the swab on a paper towel to remove excess.

c. Use the moistened cotton swab to wipe away debris. Do not try to dissolve the debris by overwetting the swab.

d. Repeat the cleaning process using additional swabs as necessary. If metallic particles are embedded in the dielectric, use an eyeglass and a sharp pick in an attempt to dislodge them. Swab again.

e. When satisfied that the interfaces are clean, blow them dry with dry compressed air, or preferably dry nitrogen (pressurized spray cans work well). Do not use breath.

f. Clean the mating connectors. These may be the source of the debris.

Appendix C
Internal Device Data Sheets

Click on link below to get internal device data sheet...

- 150 Series Programmable Attenuators...dc-18/26.5 GHz
- 3200 Series Programmable Attenuators...dc-2/3 GHz
- 3250 Series 75Ω Series Programmable Attenuators...dc-1.5 GHz
- 4226 & 4228 Series Solid-State Attenuators

Model 8311 w/Ethernet (IM-501) Revision Record

REVISION	DATE	DESCRIPTION	APPLICABLE SERIAL NUMBERS
A	8/08	Initial Issue	All Units
B	9/08	Added Models 8311-202-X-XN	New Models
C	6/09	Added Models 8311-1-X-X	New Models
D	12/09	Added Model 8311-352-9-TN	New Models
E	9/27/10	Incorporated Aeroflex / Weinschel ECN 10-237 & ECN 10-251	8310-352-9-TN
F	11/3/10	Incorporated Aeroflex / Weinschel ERN 10-180.	8310-352-12-TN
G	4/13/11	Incorporated Aeroflex / Weinschel ECN 11-079. ECN adds additional operation instructions for the Lantronix XPort™ Ethernet. Changed storage temperature range to 4° to +167 °F (-20° to +75 °C)	All Models